

NPPTL COVID-19 Response: International Respirator Assessment

Manufacturer: Fujian Yongtai Sanlian Garment CO., LTD.
Model Tested: N95 Particulate Respirator (non-medical mask)
Date Tested: August 4, 2020

These findings pertain to the Fujian Yongtai Sanlian Garment CO., LTD. model N95 Particulate Respirator (non-medical mask). The packaging for this product indicates that it meets GB2626-2006 (the Chinese standard for Respiratory Protective Equipment – Non-Powered Air-Purifying Particle Respirator).

Thirty respirators were submitted for evaluation. The respirators were sampled into groups of ten for evaluation. The samples were tested using a modified version of NIOSH Standard Test Procedure (STP) TEB-APR-STP-0059. This modified assessment plan can be found [here](#).

No certificate of approval was provided with the samples received; therefore, the authenticity of the claims cannot be validated.

The maximum and minimum filter efficiency was 99.67% and 96.91%, respectively. No respirators measured less than 95%.

NIOSH does not have knowledge about the sustained manufacturer quality system and product quality control for these products. NIOSH also does not have knowledge about the product's handling and exposures after leaving its manufacturer's control.

In addition, this product is an ear loop design. Currently, there are no NIOSH-approved products with ear loops; NIOSH-approved N95s have head bands. Furthermore, limited assessment of ear loop designs, indicate difficulty achieving a proper fit. While filter efficiency shows how well the filter media performs, users must ensure a proper fit is achieved.

This assessment is not a part of the NIOSH respirator approval process and will in no way lead to or preclude NIOSH approval through the official approval process. This assessment was developed as an assessment of the filter efficiency for those respirator's represented as certified by an international certification authority, other than NIOSH, to support the availability of respiratory protection to US healthcare workers due to the respirator shortage associated with COVID-19. Only particulate filter efficiency was assessed.

The results provided in this letter are specific to the subset of samples that were provided to NPPTL for evaluation.

These results will be used to update the CDC guidance for [Crisis Capacity Strategies \(during known shortages\)](#).

Evaluation of International Respirators

Test: Modified TEB-APR-STP-0059

Date Tested: August 4, 2020

Report Prepared: August 4, 2020

Manufacturer: Fujian Yongtai Sanlian Garment CO., LTD.

Item Tested: N95 Particulate Respirator (non-medical mask) (Sample Group 1 of 3)

Country of Certification: China (GB2626-2006)

Pictures have been added to the end of this report.

Filter	Flow Rate (LPM)	Initial Filter Resistance (mmH ₂ O)	Initial Percent Leakage (%)	Maximum Percent Leakage (%)	Filter Efficiency (%)
1	85	15.7	0.48	0.48	99.52
2	85	15.8	0.71	0.71	99.29
3	85	17.0	1.24	1.24	98.76
4	85	16.8	1.16	1.16	98.84
5	85	16.0	0.55	0.55	99.45
6	85	18.6	0.33	0.33	99.67
7	85	16.2	0.60	0.60	99.40
8	85	21.5	0.63	0.63	99.37
9	85	18.8	0.45	0.45	99.55
10	85	16.6	0.49	0.49	99.51
Minimum Filter Efficiency: 98.76%			Maximum Filter Efficiency: 99.67%		

- The test method utilized in this assessment is not the NIOSH standard test procedure that is used for certification of respirators. Respirators assessed to this modified test plan do not meet the requirements of STP-0059, and therefore cannot be considered equivalent to N95 respirators that were tested to STP-0059.
- Respirators tested may not be representative of all respirators with the same certification mark. NIOSH has no control over suppliers and distributors of respirators certified by other national or international parties.
- This assessment is not a confirmation that it conforms with any or all of its specifications in accordance with its certification mark.
- This assessment was not a part of the NIOSH approval program. These results do not imply nor preclude a future approval through the NIOSH respirator approval program.

NPPTL COVID-19 Response: International Respirator Assessment

Test: Modified TEB-APR-STP-0059

Date Tested: August 4, 2020

Report Prepared: August 4, 2020

Manufacturer: Fujian Yongtai Sanlian Garment CO., LTD.

Item Tested: N95 Particulate Respirator (non-medical mask) (Sample Group 2 of 3)

Country of Certification: China (GB2626-2006))

Filter	Flow Rate (LPM)	Initial Filter Resistance (mmH ₂ O)	Initial Percent Leakage (%)	Maximum Percent Leakage (%)	Filter Efficiency (%)
11	85	15.9	1.28	1.28	98.72
12	85	13.8	1.64	1.64	98.36
13	85	18.3	1.37	1.37	98.63
14	85	16.1	1.37	1.37	98.63
15	85	18.7	0.52	0.52	99.48
16	85	17.1	0.52	0.52	99.48
17	85	24.5	0.58	0.58	99.42
18	85	18.0	0.88	0.88	99.12
19	85	16.4	0.42	0.42	99.58
20	85	20.1	0.70	0.70	99.30
Minimum Filter Efficiency: 98.36%			Maximum Filter Efficiency: 99.58%		

- The test method utilized in this assessment is not the NIOSH standard test procedure that is used for certification of respirators. Respirators assessed to this modified test plan do not meet the requirements of STP-0059, and therefore cannot be considered equivalent to N95 respirators that were tested to STP-0059.
- Respirators tested may not be representative of all respirators with the same certification mark. NIOSH has no control over suppliers and distributors of respirators certified by other national or international parties.
- This assessment is not a confirmation that it conforms with any or all of its specifications in accordance with its certification mark.
- This assessment was not a part of the NIOSH approval program. These results do not imply nor preclude a future approval through the NIOSH respirator approval program.

NPPTL COVID-19 Response: International Respirator Assessment

Test: Modified TEB-APR-STP-0059

Date Tested: August 4, 2020

Report Prepared: August 4, 2020

Manufacturer: Fujian Yongtai Sanlian Garment CO., LTD.


Item Tested: N95 Particulate Respirator (non-medical mask) (Sample Group 3 of 3)

Country of Certification: China (GB2626-2006)

Filter	Flow Rate (LPM)	Initial Filter Resistance (mmH ₂ O)	Initial Percent Leakage (%)	Maximum Percent Leakage (%)	Filter Efficiency (%)
21	85	19.6	0.38	0.38	99.62
22	85	19.2	0.53	0.53	99.47
23	85	16.5	0.49	0.49	99.51
24	85	17.2	0.45	0.45	99.55
25	85	16.9	0.46	0.46	99.54
26	85	21.0	0.89	0.89	99.11
27	85	14.0	0.98	0.98	99.02
28	85	16.9	3.09	3.09	96.91
29	85	20.0	0.52	0.52	99.48
30	85	14.5	0.38	0.38	99.62
Minimum Filter Efficiency: 96.91%			Maximum Filter Efficiency: 99.62%		

- The test method utilized in this assessment is not the NIOSH standard test procedure that is used for certification of respirators. Respirators assessed to this modified test plan do not meet the requirements of STP-0059, and therefore cannot be considered equivalent to N95 respirators that were tested to STP-0059.
- Respirators tested may not be representative of all respirators with the same certification mark. NIOSH has no control over suppliers and distributors of respirators certified by other national or international parties.
- This assessment is not a confirmation that it conforms with any or all of its specifications in accordance with its certification mark.
- This assessment was not a part of the NIOSH approval program. These results do not imply nor preclude a future approval through the NIOSH respirator approval program.

NPPTL COVID-19 Response: International Respirator Assessment

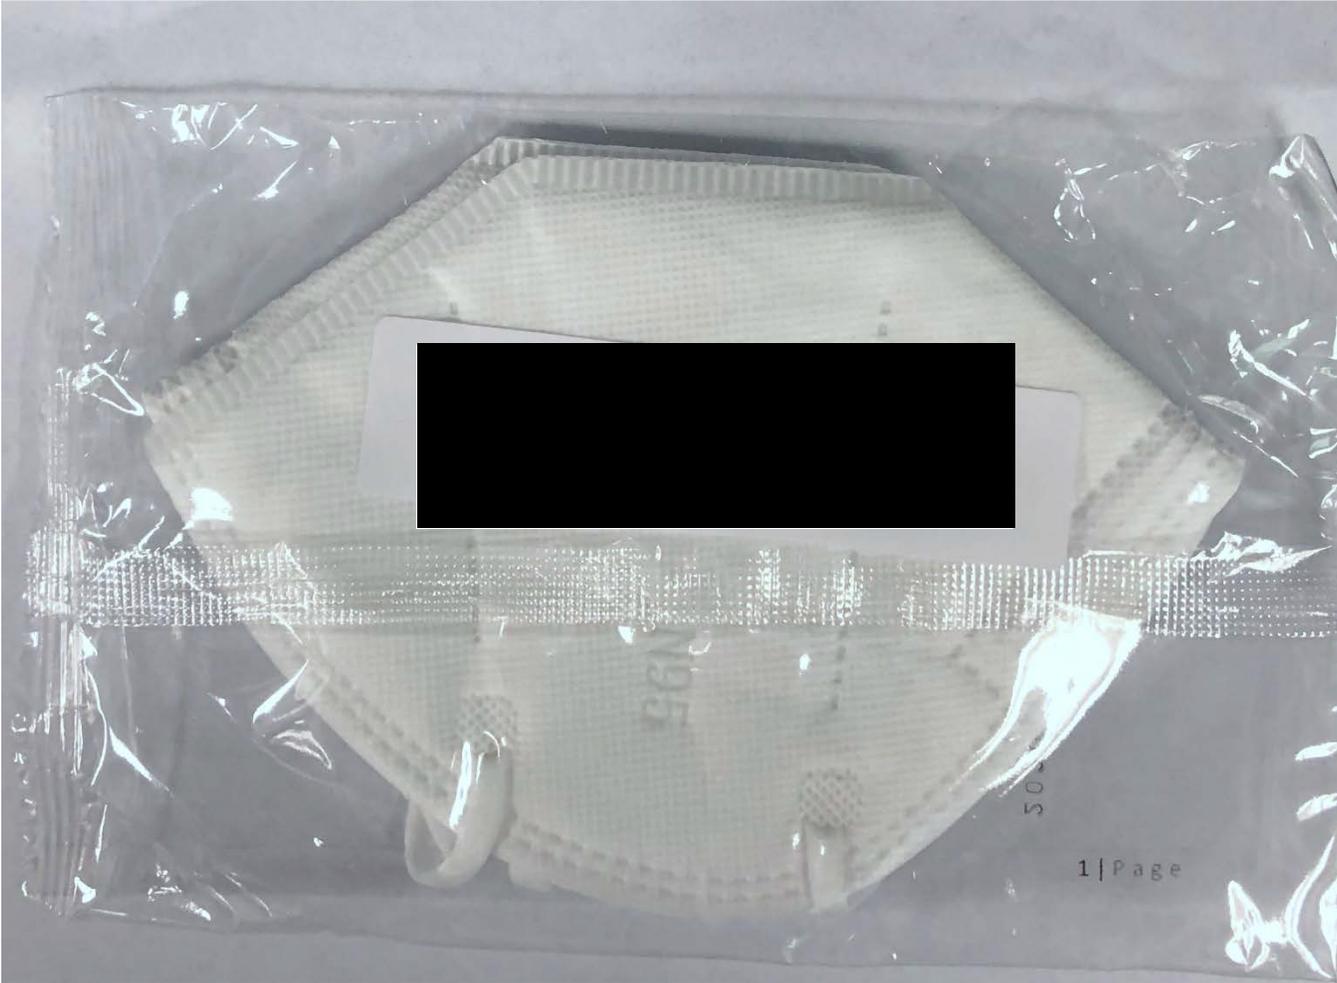

XIER

合格证

Certificate of approval

产品名称: 防颗粒物口罩(非医用口罩)

Product name: Particulate respirator (non - medical mask)

产品型号: N95

Model: N95

主要成分: 熔喷布30%、无纺布40%、
水刺棉30%

Main ingredients: melt spray cloth 30 %、 non - woven cloth 40 %、
spiny cotton 30 %

执行标准: GB 2626-2006

Implementation standard: GB 2626 - 2006

包装规格: 2个

Package size: 2 pcs

有效期: 二年

Valid: two years

生产日期: 2020.04.19

Date of production: 2020.04.19

生产批次号: 20205143

Lot number: 20205143

生产企业: 福建省永泰三连制衣有限公司

Manufacturing enterprise: Fujian yongtai sanlian garment co., ltd.

生产地址: 永泰县城峰镇马洋工业区(东洋乡厂房)

Address: Mayang Industries Zone, Chengfeng Town, Yongtai County
(Dongyang township plant), China

本产品经检验合格予以出厂

100% QC before shipment

检验: 01

Inspection: 01

NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment



NPPTL COVID-19 Response: International Respirator Assessment

