

## Review

# Nanotechnology-based electrochemical sensors for biomonitoring chemical exposures

RICHARD C. BARRY<sup>a</sup>, YUEHE LIN<sup>b</sup>, JUN WANG<sup>b</sup>, GUODONG LIU<sup>b,c</sup> AND CHARLES A. TIMCHALK<sup>a</sup>

<sup>a</sup>Biological Monitoring and Modeling Group, Pacific Northwest National Laboratory, Richland, Washington, USA

<sup>b</sup>Interfacial and Nanoscale Science Facility, Pacific Northwest National Laboratory, Richland, Washington, USA

<sup>c</sup>Department of Chemistry and Molecular Biology, North Dakota State University, Fargo, North Dakota, USA

The coupling of dosimetry measurements and modeling represents a promising strategy for deciphering the relationship between chemical exposure and disease outcome. To support the development and implementation of biological monitoring programs, quantitative technologies for measuring xenobiotic exposure are needed. The development of portable nanotechnology-based electrochemical (EC) sensors has the potential to meet the needs for low cost, rapid, high-throughput, and ultrasensitive detectors for biomonitoring an array of chemical markers. Highly selective EC sensors capable of pM sensitivity, high-throughput and low sample requirements ( $< 50 \mu\text{l}$ ) are discussed. These portable analytical systems have many advantages over currently available technologies, thus potentially representing the next generation of biomonitoring analyzers. This paper highlights research focused on the development of field-deployable analytical instruments based on EC detection. Background information and a general overview of EC detection methods and integrated use of nanomaterials in the development of these sensors are provided. New developments in EC sensors using various types of screen-printed electrodes, integrated nanomaterials, and immunoassays are presented. Recent applications of EC sensors for assessing exposure to pesticides or detecting biomarkers of disease are highlighted to demonstrate the ability to monitor chemical metabolites, enzyme activity, or protein biomarkers of disease. In addition, future considerations and opportunities for advancing the use of EC platforms for dosimetric studies are discussed.

*Journal of Exposure Science and Environmental Epidemiology* (2009) **19**, 1–18; doi:10.1038/jes.2008.71; published online 19 November 2008

**Keywords:** biomonitoring, dosimetry, electrochemical sensors, exposure assessment.

## Introduction


Biological monitoring (biomonitoring) has the ability to integrate total chemical exposure to assess human dosimetry (Yantasee et al., 2007a). This includes exposure from multiple sources (i.e., air, soil, water, and food residues) and multiple routes of intake (i.e., inhalation, oral, and dermal). A benefit of biomonitoring is the ability to associate the internal dose of a given chemical or metabolite with a measurable effect (either tissue specific or whole body), which can then be used for risk assessment purposes (Friberg and Elinder, 1993; Christensen, 1995; Gilbert and Sale, 2005). Likewise, biomonitoring can be exploited to distinguish between internal (actual) from potential exposure. As

suggested by Angerer et al. (2006) and illustrated in Figure 1, the exposure–effect continuum represents a framework for assessing chemical exposures and making both risk assessment and management decisions within epidemiological studies. In this regard, it is suggested that the most meaningful interpretation of epidemiology studies could be realized by accurately assessing chemical exposure with biological effect. However, a major impediment to conducting epidemiology studies is the lack of affordable quantitative technologies that can readily measure chemical exposure markers (biomarkers) using minimally invasive biological fluids (Weis et al., 2005). To address these limitations, inexpensive microanalytical-based sensors are needed that can accurately and precisely process small amounts of biological fluids. Ideally, these sensors can be used for parallel analyses of multiple markers or quickly adapted for detection of a broad range of biomarkers associated with chemical exposure and biological response (Liu et al., 2005; Weis et al., 2005). As reviewed by Weis et al. (2005), microsensor platforms offer great promise because they have the potential to provide rapid, accurate, and quantitative detection of exposure at the level of the individual. The data

1. Address all correspondence to: Dr. Charles A. Timchalk, Biological Monitoring and Modeling Group, Pacific Northwest National Laboratory, MSIN: P7-59, 902 Battelle Blvd., Richland, WA 99352, USA. Tel.: +1 509 376 0434. Fax: +1 509 376-9064.

E-mail: charles.timchalk@pnl.gov

Received 21 February 2008; revised 30 July 2008; accepted 23 September 2008; published online 19 November 2008

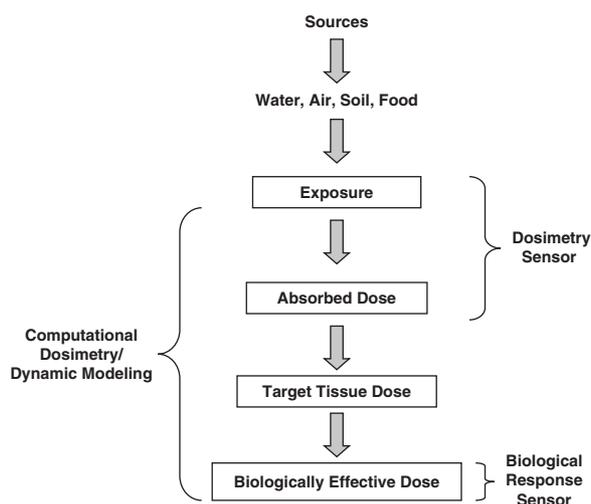

**Figure 1.** Diagram of the exposure–effect continuum relating exposure source with dosimetric and biological response. Figure adapted from Angerer et al. (2006).

generated from such devices can then be used to effectively couple environmental and personal exposure assessment in a way that enhances our ability to study the factors that affect health and disease across large populations.

The identification and quantification of target chemicals or their metabolites in biological fluids (blood, urine, and saliva) is still a cornerstone of xenobiotic metabolism research, where the analytes represent the key biological monitoring targets (Gil and Pla, 2001; Angerer et al., 2006). However, the utility of a specific analyte (e.g., chemical metabolite) for quantitative biological monitoring requires an appreciation of its pharmacokinetics; that is, a concentration associated with the rate of absorption, distribution, metabolism, and/or excretion in the relevant biological matrices (Timchalk et al., 2001, 2004a,b). A strategy for the development, validation, and deployment of a chemical biomonitoring platform is illustrated in Figure 2. Key criteria include identification of markers in complex matrices, such as blood, urine or saliva, validation of sensor performance, and deployment of a user-friendly platform. Validation should not only include characteristics of instrument performance (e.g., limit of detection, limit of quantification, linear performance, reproducibility, matrix effects, etc.), but the marker(s) should have positive predictive value that link chemical exposure with adverse health effects.


This review is focused on the development and validation of portable electrochemical (EC) sensors that incorporate nanomaterials as either a signal transducer or as an electroactive species for indirect detection of analyte. Given the sensitivity, flexibility, and miniaturization capabilities, these sensors have the potential to become the next generation of field-deployable analytical instruments. Our intent is to: (1) provide a general overview of EC terminology, detection methods, and integrated use of

nanomaterials in the development of EC-based microanalytical instrumentation; (2) highlight recent developments using EC sensors for biomonitoring; (3) illustrate recent applications of nanotechnology-based EC sensors for detection and quantification of biomarkers of exposure or disease; and (4) discuss future considerations and opportunities for advancing the use of EC sensors for dosimetric studies.


## Methods

### *Review of General Terms and Overview of Electrochemical Sensors*

EC measurements are based on detection or transport of charge across an electrode. Chemical species, such as molecular ions, are referred to as electroactive species if they can either be oxidized (lose electrons) or reduced (gain electrons) at an electrode surface through the movement of electrons. A detector that measures current when an electroactive solute contacts a working electrode held at a fixed potential with respect to a reference electrode is known as an amperometric detector; whereas measurement of current that develops as a function of variable potential is known as voltammetry. In voltammetry, a variable potential excitation signal is impressed upon a solution through an electrode to generate a characteristic signal at the electrode, known as waveforms and expressed as potential per unit time. Amperometric and voltammetric detectors both generate quantitative information of electrode current *versus* time, but voltammetry has the added advantage of providing characteristic current response information for reversible reactions by pulsing an applied potential between high and low values. If the added potential is pulsed with short-time intervals between high and low values, the current that flows back and forth through the electrode can be measured during the lifetime of the pulse. As the potential is pulsed in voltammetry between high and low voltage values, the analyte (or product) at the surface of the electrode can undergo a corresponding reduction or oxidation and generate positive or negative current flow. A plot of the difference between the changing current flows ( $\Delta i = i_{\text{highV}} - i_{\text{lowV}}$ ) *versus* potential results in a voltammogram that is characteristic for the electroactive species (Skoog and Leary, 1992). When the potential is applied in a staircase fashion a waveform is produced (potential per unit time) and the technique is known as square-wave voltammetry. In stripping analysis, the solute is preconcentrated (electrodeposited) at the surface of the electrode using a constant applied potential before application of a stripping potential (stripping voltammetry) to redissolve the material from the electrode (Figure 3). If the stripping potential is applied as a square wave, the technique is known as square wave stripping voltammetry. Classical amperometric and voltammetric EC methods have been attractive as analytical techniques because they offer

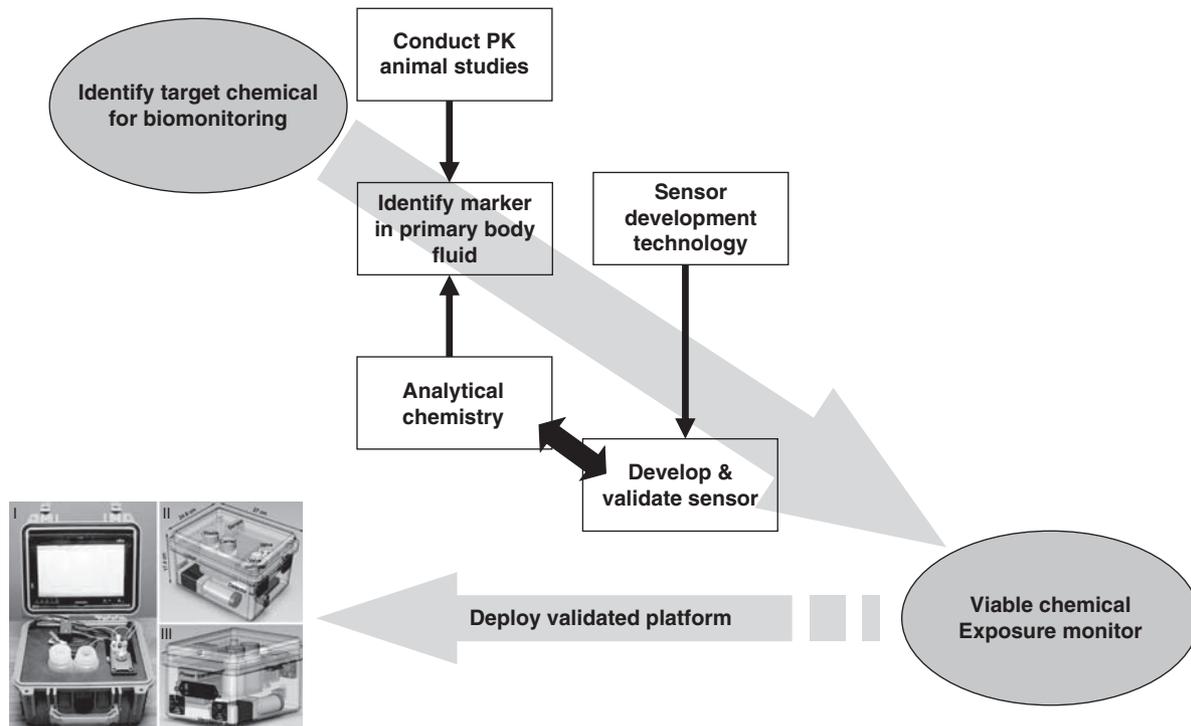


**Figure 2.** Strategy for the development, validation, and deployment of biological monitoring sensor platforms.

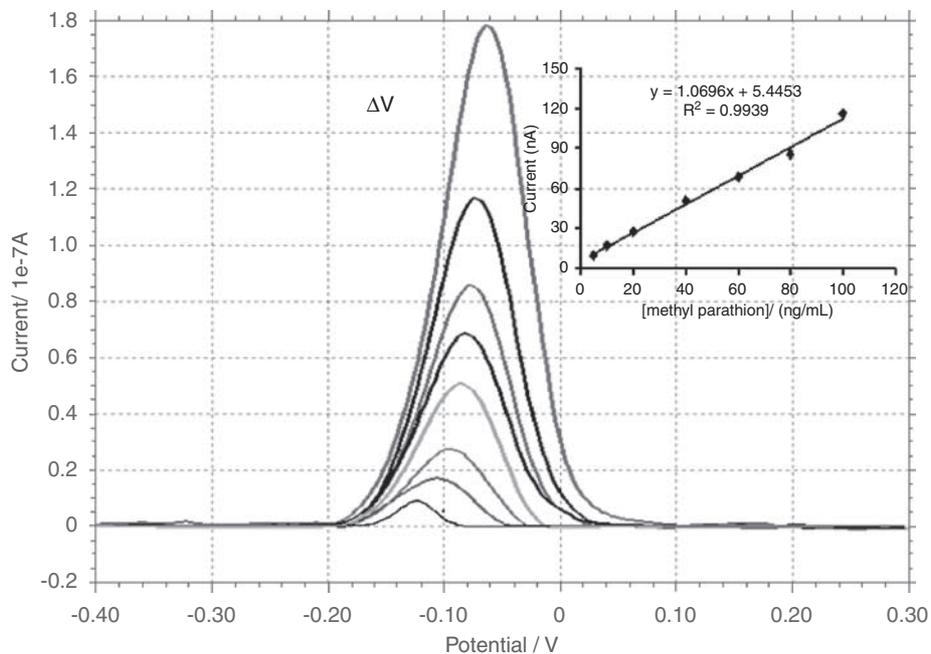

**Figure 3.** Stripping voltammograms, current *versus* applied potential, of increasing methyl-parathion (pesticide) concentration, from bottom to top, 5, 10, 20, 40, 60, 80, 100, and 200 ng/ml. The inset shows the calibration curve (adapted from Liu and Lin, 2005).

detection limits on the order of  $10^{-7}$  or  $10^{-8}$  M, whereas stripping analysis preconcentrates solutes to achieve limits down to  $10^{-10}$  to  $10^{-11}$  M (Bard and Faulkner, 1980). As

many analytes are electroactive, EC methods are the most widely used alternatives to atomic and/or mass spectroscopic techniques for trace detection of analytes.

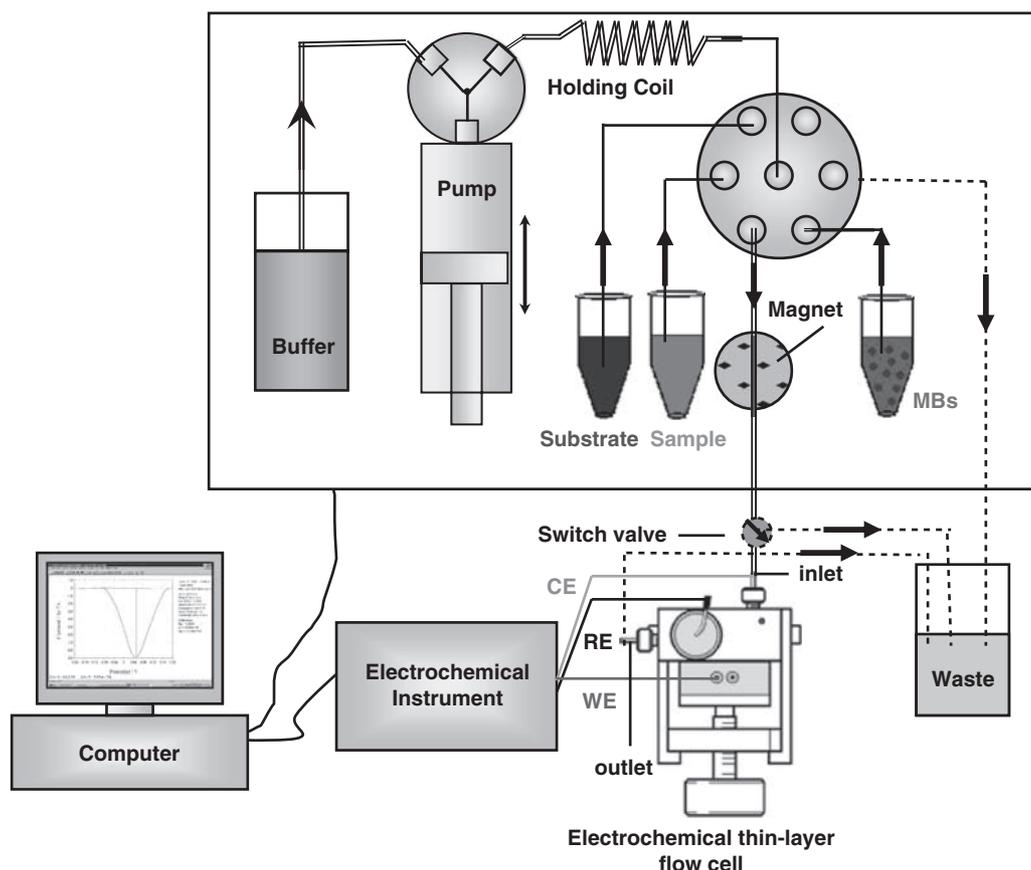

**Figure 4.** Schematic of sequential injection/electrochemical immunoassay for quantification of 3,5,6-trichloro-2-pyridinol (TCP). The computer-controlled sequential-injection analysis system (MicroSIA; FIALab Instruments Inc., WA, USA) includes six-port selection valve for delivering sample and reagents, a thin-layer cross-flow cell (MF-1095; Bioanalytical system Inc., West Lafayette, IN, USA) that contains a glassy carbon electrode, a Ag/AgCl reference electrode and electrochemical analyzer voltammetric detection of electroactive species (Model CHI 660; CH Instruments Inc., TX, USA). Figure adapted from Liu et al. (2005) with permission.

EC methods are also more amenable to the development of portable instrumentation because of their simplicity, low power requirements, and ability to be miniaturized. Techniques that are based on manipulation of a liquid sample have been particularly fruitful for detection of toxic chemicals, these include flow-injection analysis and sequential-injection analysis using amperometric detection (Neufeld et al., 2000; Sole and Alegret, 2001; Gilbert and Sale, 2005; Xu et al., 2007), and microelectrical mechanical systems (Wang et al., 2001; Chen et al., 2006a). In each of these injection methods, samples are injected into flow cells and transported by a carrier solution and reacted with select substrates that can be electrochemically detected (Figure 4). By using a calibration curve, analyte concentration can be calculated from the detector response. Flow-injection analysis with amperometric detection, for example, offers the possibility of real-time and continuous-flow detection of toxic compounds within environmental or biological samples, using very small volumes ( $<20 \mu\text{l}$ ) or high-throughput analysis of numerous samples (3600 injections per h) (Wang and Li, 1990;

Liu et al., 2005; Liu and Lin, 2006). Microfabrication technology has been used to develop wholesale separations and detection on a single microelectrical mechanical systems microchip. Most fabrication processes involve photolithography, wet etching, laser ablation, or injection molding to form microchannels, valves, and interconnects on silicon, glass, or polymer substrates (Manz et al., 1991; Belmont et al., 1996; Chen et al., 2006a). Fluid flow or analyte detection is then carried out by electrical methods. Amperometric and conductivity detection have used microelectrical mechanical devices, for example, for the detection of various residues of chemical nerve agents (Wang et al., 2001), nitroaromatic compounds (Wang et al., 2002), and heavy metal ions (Collins and Lu, 2001; Dabek-Zlotorzynska et al., 2003).

Even with the tremendous inventiveness exhibited by numerous researchers, the application of EC methods has been limited because of the need for electrodes with unique electrical and selective properties. However, new developments in material science have now produced a broad range

of technologies that are being adapted to increase the utility of EC sensors.

#### *Modern Advances in the Development of Electrochemical Sensors*

Recent advances in printing technology and materials science now allows greater flexibility in producing extremely inexpensive, reliable, and selective electrodes for detection of specific analytes. These advances can be grouped into three EC technologies: screen-printed electrodes, integrated nanomaterials, and EC immunoassays. Hybrid devices that incorporate the advantages of each of these new technologies are also being developed. In general, modern advances in the development of low cost and selective EC sensors offer a greater range of applications for analysis of chemical exposure for environmental or biological monitoring. These systems are suitable for the determination of chemicals, metabolites, proteins, metals, inorganic ions, organic compounds, and other biological molecules in a variety of biological matrices.

#### *Screen-Printed Electrodes*

Various types of carbon-based, plastic, and ceramic materials are being coated with different doping agents to enhance electron transfer or coated with selectivity agents to capture analytes of interest using screen-printing technology (e.g., photolithography). The coated electrodes are then employed as the working electrode in voltammetric analyses (Badihi-Mossberg et al., 2007; Renedo et al., 2007). The coatings may include agents such as metals, complexing molecules, immobilized enzymes, or affinity agents (e.g., antibodies). Screen-printed electrodes can be categorized according to how the electrode is modified: metal-modified, enzyme-modified, or affinity capture-modified (Renedo et al., 2007). Electrodes doped with gold or silver atoms, or coated with gold, mercury, bismuth, or nickel metal films have been used with stripping voltammetry to monitor a variety of hazardous metals and chemicals in biological fluids with detection limits of ng/ml; enzyme-immobilized screen-printed electrodes have been used to detect enzyme activity, pesticide metabolites, phenolic compounds, heavy metals, cholesterol, and glucose in biological matrices by immobilizing an enzyme onto a sol-gel matrix or conductive polymer to ng/ml levels; whereas antibody-immobilized screen-printed electrodes have been used with amperometric and voltammetric detection of antigen in biomatrices at the pg/ml level (Renedo et al., 2007). For a comprehensive review of the latest applications of screen-printed electrodes, see Renedo et al. (2007).

#### *Integrated Nanomaterials for EC Applications*

The advent of nanotechnologies has led to enormous advances not only in basic science but also in detection strategies. Nanomaterials offer new platforms for developing a variety of advanced analytical technologies, including more

sensitive and selective EC sensors for biomonitoring. The most studied nanomaterials, carbon nanotubes, metal nanoparticles, and quantum dots (QDs) have been especially targeted for developing novel biosensors (He and Toh, 2006; Liu and Lin, 2006; Pumera et al., 2007; Liu et al., 2007a,b; Wu et al., 2007a,b). Nanomaterials are now being used as signal transducers to mediate current flow or as electroactive tags to indicate the detection of analyte.

Nanomaterials are attractive because of their unique electrical, chemical, and physical properties (i.e., size, composition, conductivity, magnetism, mechanical strength, light absorbing, and emitting properties). Carbon nanotubes, colloid gold, QDs, and zirconium oxide nanoparticles have all been used for EC detection of chemicals in the environment and more recently in biological samples (Liu and Lin, 2005, 2006; Kim et al., 2007; Wang et al., 2008a,c). By utilizing nanomaterials, EC biosensors have shown great promise for detection of chemical markers and biomarkers of exposure primarily because the nanomaterials are used to either capture the marker or amplify the signal associated with detection. Both of these capabilities are important for trace level detection in complex biological matrices. Two approaches are currently used for nanomaterials-based EC biosensors: (1) the use of nanomaterials as the electrical signal transducer and (2) nanomaterials used as electroactive tags for the indirect detection of analyte. Carbon nanotubes and metal nanoparticles have, for example, been used to modify the electrode surface for enhancing EC response due to their electrocatalytic properties (Chen et al., 2007). In addition, silicon nanowires and conducting polymer nanowires have been used as field-effect transistors (Patolsky et al., 2006). Alternatively, some nanoparticles are used as the electroactive reporters for indirect detection of analyte and/or for signal amplification purposes; the most common of which are metal (e.g., colloid gold) and inorganic nanoparticles (e.g., Fe<sub>2</sub>O<sub>3</sub> and CdSe QDs) (Authier et al., 2001; Cui et al., 2007; Wu et al., 2007a,b; Liu et al., 2007b). Collectively, EC assays that integrate nanomaterials have been used for the detection of chemical exposure or biomarkers of disease using a variety of biological matrices (Wang et al., 2003, 2006a; Liu and Lin, 2005, 2006).

Carbon nanomaterials contain nanostructures that seem to be especially suitable for the development of EC biosensors (Tasis et al., 2006). In particular, carbon nanotubes and carbon nanofibers possess conductivity, surface areas, chemical functionalities, and biocompatibility that make them ideal for the development of compound-specific biosensors (Andrescu and Marty, 2006; Trojanowicz, 2006; Du et al., 2007; Kim et al., 2007). Carbon nanotubes are composed of graphite carbon with one or more concentric tubes. Recent studies have shown that carbon nanotubes can enhance the direct electron transfer reactions of some biomolecules, including cytochrome *c*, catalase, and nicotinamide adenine dinucleotide due to the unique electronic

structure, electrical conductivity, and high surface area available on carbon nanotubes for redox reactions (Lin et al., 2005; Liu and Lin, 2006; Wang et al., 2006b, 2008a).

Nanoparticles such as colloidal metals (e.g., gold or silver), inorganic crystals (e.g., QDs), and silica are currently being used as labels, markers, or probes for detection of a wide-range of biomolecules (Guo and Wang, 2007). In most cases, these types of nanoparticles are conjugated to some biomolecule (e.g., DNA, protein, or antibody) and the biomolecule is used for identifying certain biomolecular interactions, cellular translocations, or affinity capture of an analyte of interest. The most common approaches use colloidal gold or QDs as the electroactive species. QDs are nanoscale crystals composed of group II–VI or III–V elements (e.g., CdSe, ZnS, or Fe<sub>2</sub>O<sub>3</sub>) that can either absorb light energy and emit photons at characteristic wavelengths (Jamieson et al., 2007; Wang et al., 2008b) or be acid solubilized to generate electroactive metal ions (Wu et al., 2007a,b; Liu et al., 2007b). A variety of EC DNA sensors, for example, have been functionalized with nanoparticles for direct and indirect detection of metal ions, proteins, RNA, and DNA, with detection limits as low as zeptomoles (10<sup>-21</sup> mol) (Authier et al., 2001; Drummond et al., 2003; Liu and Lu, 2003; Wang et al., 2003; Tansil and Gao, 2006). Nanoparticle-based EC bioassays for proteins have been reviewed by Wang (2007). There are also considerable efforts to leverage nanoparticle sensitivity with antibody selectivity using EC methods, known as EC immunoassays.

### *Electrochemical Immunoassays*

Immunoassay-based sensors have been developed to exploit the high degree of specificity and affinity of antibodies for specific antigens (Liu et al., 2007a,b; Wu et al., 2007a,b). In this particular application, a given chemical, metabolite, or modified protein can act as the antigen, and an EC response linked to antibody binding with the antigen. Generally, the antibody or analyte of interest is immobilized on a membrane, magnetic bead, or EC transducer, and the analyte is measured by signal derived from a conjugated tag that is attached to either the antibody or analyte. Two types of immunoassays are generally employed: a competitive active site assay or the sandwich assay. In the competitive immunoassay, the analytes within a matrix compete with an analog analyte for antibody sites and the signal from the analog is used to calculate how much analyte of interest was captured. The analog is labeled or tagged in some fashion (e.g., enzyme or nanoparticle), and it is the tag that ultimately generates detectable electroactive species. In this assay, the amount of analyte present is calculated by determining the ratio of analog signal relative to the known maximum amount of signal possible for a known concentration of analog (Lin et al., 2007; Zacco et al., 2007). The second type of immunoassay utilizes a primary antibody to selectively capture the analyte from the matrix and a

secondary antibody containing a signaling device to quantify the captured analyte. The two antibodies effectively sandwich the analyte in between them and the approach is referred to as a sandwich immunoassay. Conventionally, enzymes are conjugated on the secondary antibody and used to generate signal in the biological technique known as enzyme-linked immunosorbent assay (ELISA). With the addition of substrate (unrelated to the analyte) the enzyme selectively cleaves the substrate to generate signal (i.e., light, fluorescence, ions, etc.). With EC assays, tags that generate electroactive species are ideal and a variety of nanomaterials are being evaluated as potential tags when conjugated to antibodies. Metal nanoparticles such as colloidal gold or CdSe QDs are typically used, and commercial kits are available for conjugation to antibodies (Knecht et al., 1986; Hainfeld and Powell, 2000; Merkoci et al., 2005; Jain, 2007; Wang, 2007). On the basis of these approaches, several immunosensors have been developed for the detection of a range of xenobiotics and protein biomarkers of disease including: the herbicide chlorsulphuron, polychlorinated biphenyls, polycyclic aromatic hydrocarbons, 2,4,6-trichloroanisole, pesticide metabolites, human myoglobin, cardiac troponin, and creatine kinase (Velasco-Arjona et al., 1997; Galve et al., 2002; Piras and Reho 2005; Liu et al., 2005, 2006; Dong et al., 2007; Renedo et al., 2007). EC immunoassays routinely achieve detection limits in the low pM range and three orders of dynamic range using < 50 μl of sample.

## **Results**

### *EC Sensors for Biomonitoring*

There have been a number of recent overviews discussing advances in the application of EC sensors for industrial hygiene and environmental monitoring (Ashley, 2003; Hanrahan et al., 2004), as well as the development of personal exposure biomonitoring for heavy metals (Yantasee et al., 2007a,b) and ChE biosensors (Andreescu and Marty, 2006). As reviewed by Ashley (2003), EC sensors have been developed for field monitoring of a broad range of chemical contaminants including: inorganic gases and vapors (carbon monoxide, carbon dioxide, sulfur dioxide, nitric, and nitric oxide), volatile organic hydrocarbons, aldehydes and ketones, heavy metals, pesticides, and some persistent pollutants. However, as noted by Weis et al. (2005) the utilization of these sensors for human studies and in particular biological monitoring has not yet been fully realized.

Considerable effort has also been made to develop sensor platforms that monitor toxic metals or chemical xenobiotics in environmental applications (i.e., in air, water, or soil) (Sadik and Van Emon, 1996; Sole and Alegret, 2001; Hanrahan et al., 2004), but there is a general lack of publications that specifically focus on the detection and

quantification for human biomonitoring. It is important to note that in some cases sensor systems that have been developed for environmental monitoring may be utilized with biological samples with minimum validation; but in other cases methods must be dramatically modified to instead detect a metabolic byproduct or avoid fouling of the sensor due to matrix effects. For example, a number of EC-based sensor platforms have been developed for the detection of the phenoxyacetic acid herbicide 2,4-D in a range of environmental media (Kröger et al., 1998; Haláamek et al., 2001; Kim et al., 2007). In the case of human biomonitoring, 2,4-D is readily absorbed and excreted primarily unchanged in the urine (Arnold and Beasley, 1989; Timchalk 2004); hence, the primary issue for adapting the environmental sensor systems for human biomonitoring is to optimize performance for urine matrix effects and validate the sensor against biological samples (i.e., urine) containing 2,4-D. In other cases it may not be feasible to directly adapt environmental sensors for human biomonitoring, particularly in those situations where the environmental chemical undergoes extensive *in vivo* metabolism. In all cases, however, field trials will be required to validate the EC sensor performance against conventional methods. Recently, Yantasee et al. (2007a,b) performed validation studies of nanotechnology-based capture of toxic metals from biological matrices and subsequent quantification using EC methods. Results from a lead dosing study of rats demonstrated that the EC sensor was capable of detection limits of 0.44 and 0.46 p.p.b. with %RSD of 4.9 and 2.4 in 50% urine and 10% blood, respectively (Yantasee et al., 2007b). The sensor results were very similar to lead concentration values as measured by ICP MS, but EC sensor data were generated within 3 min per sample using 60  $\mu$ l of matrix whereas ICP MS required considerably more sample preparation.


#### *Biomarkers of Organophosphate Pesticide Exposure*

Considerable efforts are also being made to develop EC sensors that can be used for biomonitoring of pesticide biomarkers. Organophosphorus insecticides constitute a large class of chemical pesticides that are widely used (Aspelin, 1992, 1994) and have been involved in more poisoning cases than any other single class of insecticide (Al-Saleh, 1994). These chemicals have a high affinity for binding to and inhibiting the enzyme acetylcholinesterase (AChE), an enzyme specifically responsible for the destruction of the neurotransmitter acetylcholine (ACh) within nerve tissue (Ecobichon, 2001). As the cholinergic system is widely distributed within both the central and peripheral nervous systems, chemicals that inhibit AChE are known to produce a broad range of well-characterized symptoms (for review see Savolainen, 2001). A comparison of the AChE inhibition dynamics for the interaction of ACh, and the “active” insecticide metabolite chlorpyrifos-oxon (organophosphate) with AChE is illustrated as an example in Figure 5. Both

substrates have relatively high affinities for AChE and readily complex with the enzyme; however, the rates of hydrolysis and reactivation of AChE following phosphorylation of the active site will be drastically slower than for the hydrolysis of the acetylated enzyme (Ecobichon, 2001). For organophosphorus insecticide biomonitoring, sensor development has mainly focused on the measurement of ChE activity and quantification of major metabolites. Current efforts are also underway in our laboratory to detect the organophosphate chemical adducts that preferentially form on proteins (e.g., ChE) in the relevant biological matrices. Biomonitoring offers one of the best approaches for accurately assessing human dosimetry and for determining risk from chemical exposures (Friberg and Elinder, 1993; Christensen, 1995; Timchalk et al., 2001, 2007a,b). In the case of organophosphorus insecticides, blood and urine have been the primary matrices for evaluation of both dosimetry (parent and metabolites) and ChE activity (Peoples and Knaak, 1982; Nolan et al., 1984; Chester, 1993; Timchalk et al., 2002). However, other matrices such as saliva are being investigated and may offer a single non-invasive matrix for assessing both ChE activity and dosimetry (Borzelleca and Skalsky, 1980; Ryhanen, 1983; Kousba et al., 2003; Henn et al., 2006; Timchalk et al., 2004, 2007a).

Diethylphosphorothionates, for example, are one of the major subclasses of organophosphorus insecticides, which include a number of commonly used pesticides, such as chlorpyrifos, diazinon, and parathion. A representative scheme (Figure 6) for the metabolism of chlorpyrifos shows that it undergoes CYP450-mediated oxidative desulfation or dearylation to form chlorpyrifos-oxon (the neurotoxic moiety) or 3,5,6-trichloro-2-pyridinol (TCP) and diethylthiophosphate, respectively (Chambers and Chambers, 1989; Ma and Chambers, 1994). Hepatic and extrahepatic esterases such as paraoxonase and cholinesterase effectively metabolize chlorpyrifos-oxon to form TCP and diethylphosphate. Dialkylphosphates, such as diethylphosphate and diethylthiophosphate, have long been used as general urinary biomarkers for this class of insecticides (Hardt and Angerer, 2000; Bradman et al., 2005; CDC, 2005; Timchalk et al., 2007b). For assessing human exposure to specific organophosphorus insecticides, the metabolite containing the organic moiety, such as TCP in the case of chlorpyrifos, has been used as this is a specific biomarker found in urine (Nolan et al., 1984; Barr et al., 2004; Berkowitz et al., 2004; Eskenazi et al., 2004; CDC, 2005; Timchalk et al., 2007b).

In addition, the chemical reactivity and covalent binding of organophosphorus insecticides and nerve agents with blood and tissue proteins produce novel chemical adducts (known as alkylphosphorylation and simply referred to as phosphorylation) on specific matrix proteins that have the potential to be exploited as biomarkers of exposure. The most common modification is phosphorylation of cholinesterase (either AChE or butyrylcholinesterase) and subsequent inactivation

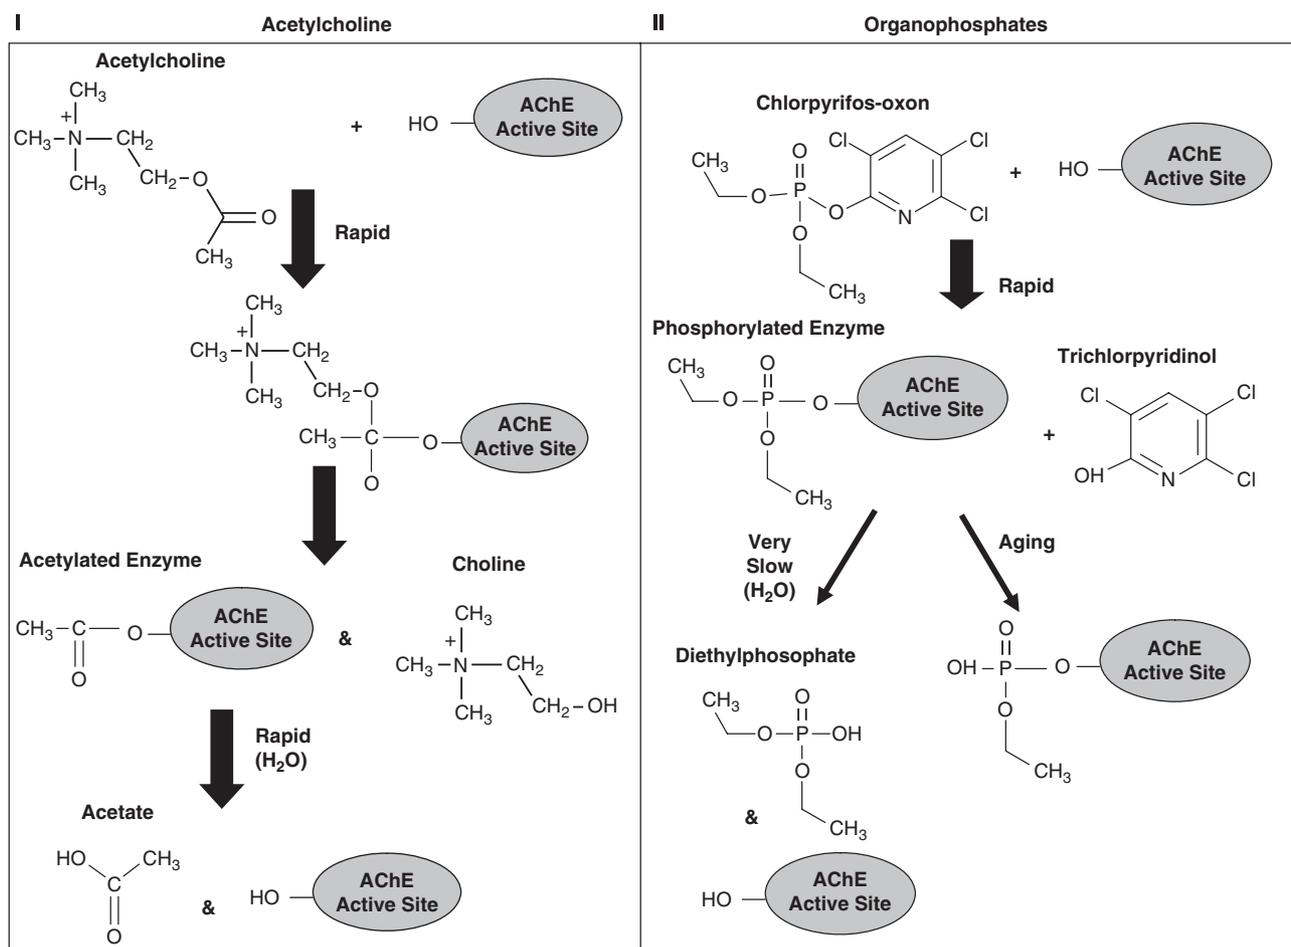


**Figure 5.** Schematic illustrating the interaction of acetylcholine (ACh) (I), and the organophosphate chlorpyrifos-oxon (II) with the active site of acetylcholinesterase (AChE).

of cholinesterase, leading to cholinergic system failure. Phosphorylated adducts have also been detected on other proteins, including carboxylesterase, neuropathy target esterase, trypsin, chymotrypsin, and human serum albumin (Ooms and van Dijk, 1966; Boter and Ooms, 1967; Ecobichon and Comeau, 1973; Johnson, 1975; Fonnum et al., 1985; Johnson and Glynn, 1995; Black et al., 1999; Elhanany et al., 2001; Peeples et al., 2005; Li et al., 2007). Biomonitoring of protein adducts extends the time interval between exposure and sampling and may be a suitable approach to detect low-level exposure. In this regard, Polhuijs et al. (1997) developed a procedure for the analysis of phosphorylated binding sites, which is based on reactivation of the phosphorylated enzyme with fluoride ions. On the basis of these methods, it was suggested that detection levels in the range of ~0.01% inhibited butyrylcholinesterase should be quantifiable. This represents a detection level that is several orders of magnitude greater than what is currently possible on the basis of measuring cholinesterase

activity. Thus, three different types of biomarkers of OP exposure are available which can be used to provide information as to the subclass of pesticide involved (e.g., organophosphate *versus* carbamate), extent of exposure, and used to determine the association with adverse health: cholinesterase activity, chemical metabolites, and phosphorylated protein.

#### Applications of EC Sensors for Biomonitoring AChE Activity

The utility and advantage of using carbon nanotubes in EC biosensors is demonstrated below in two examples that seek to monitor biological enzyme activity as a way to assess chemical exposure. Each uses an enzyme immobilized on a screen-printed carbon nanotube electrode but one type is for the direct detection of substrate hydrolysis products, whereas the other is an indirect method that relies on a redox (electron exchange) reaction to generate hydrogen peroxide (H<sub>2</sub>O<sub>2</sub>).

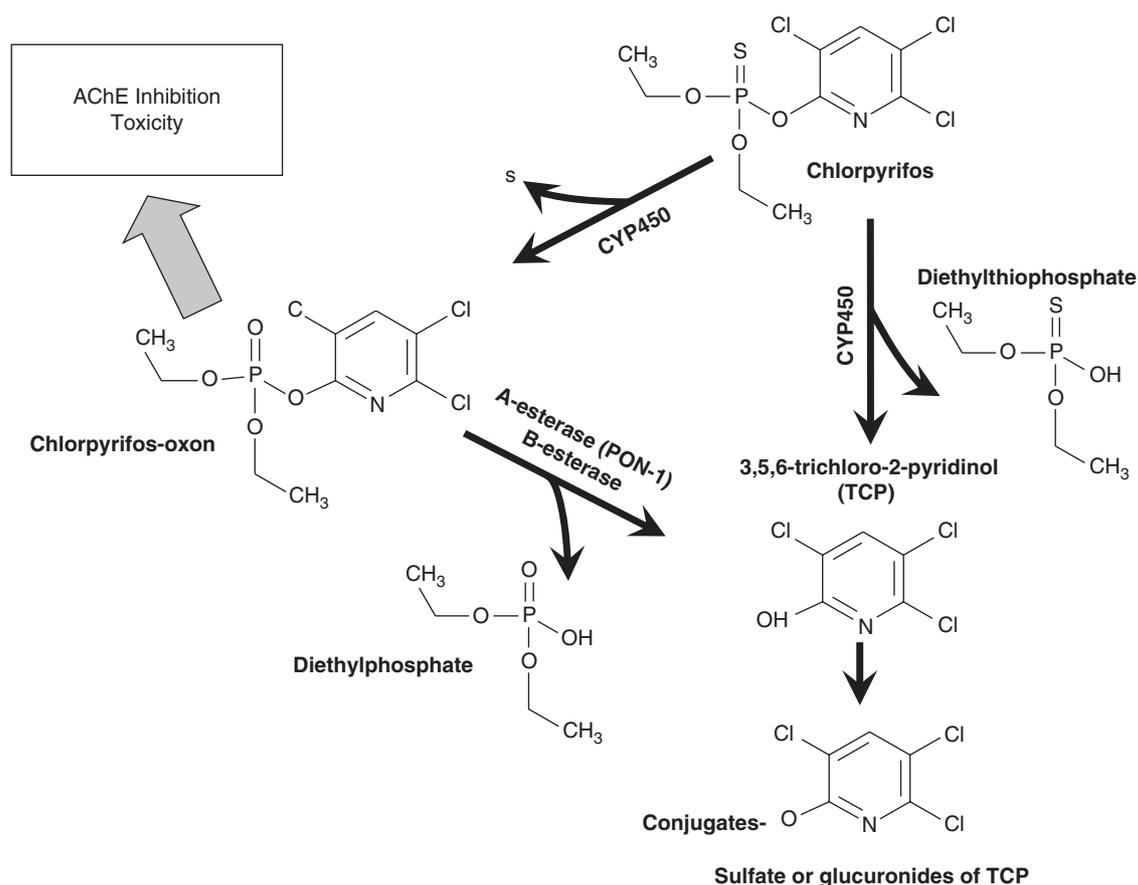


**Figure 6.** Metabolic scheme for the metabolism of chlorpyrifos and the major metabolites chlorpyrifos-oxon, trichloropyridinol (and conjugates), diethylphosphate and diethylthiophosphate. Figure adapted from Timchalk et al. (2004a,b) with permission.


Generally, two approaches have been used for characterization of cholinesterase activity in biological matrices using carbon nanotube-based EC biosensors: either a single-step system utilizing indigenous cholinesterase and appropriate substrate (Liu and Lin, 2006) or a binary method where cholinesterase is combined with choline oxidase (ChO) to generate and detect  $H_2O_2$  as an electroactive end product (Guerrieri and Palmisano, 2001; Lin et al., 2004). The cholinesterase activity in either system is monitored by measuring the oxidation or reduction current of the product of the enzymatic reaction(s).

The first example of a cholinesterase-immobilized screen-printed electrode reaction series is shown in Eqs. (1) and (2) (Liu and Lin, 2006). In this sensor, AChE was self-assembled on top of a carbon nanotube (graphite carbon) surface and integrated with a flow injection system using amperometric monitoring for the detection of hydrolyzed acetylthiocholine substrate. The carbon nanotube acts in this case as both a convenient platform for enzyme immobilization and efficient electron transducer to monitor inhibition of the enzyme in the presence of the pesticide paraoxon. The single-step reaction involved AChE hydrolysis of a known

amount of acetylthiocholine substrate:




The subsequent oxidation of the thiocholine (TCh) at the electrode surface gives rise to a current that constitutes a quantitative measurement of the enzymatic activity:



As AChE activity is inversely related to the amount of paraoxon present in the system, the sensor can be used for quantification of inhibitor present in the matrix. This sensor was sensitive to sub pM levels (pg/ml) of paraoxon and 20% AChE inhibition after six minutes of exposure (incubation) using  $20 \mu\text{l}$  of sample.

In some cases, it may be necessary to indirectly detect enzyme inhibition by adding reagents that are more amenable for detection by EC methods. In the following binary enzyme system (Eqs. (3) and (4)), AChE enzymatically cleaves the neurotransmitter ACh *in vivo* into acetate and choline, and

choline is subsequently converted to an aldehyde and hydrogen peroxide ( $\text{H}_2\text{O}_2$ ) by ChO for the amperometric detection of  $\text{H}_2\text{O}_2$  (Lin et al., 2004):



For this system, the carbon nanotube-EC method produced a detection limit of 50 nM organophosphate pesticide and a sensitivity of 0.48% inhibition/ $\mu\text{M}$  enzyme (Lin et al., 2004).


In both of the carbon nanotube sensor examples, the presence of any chemical inhibitor of AChE, such as an organophosphate pesticide, would lead to lower current measurements. A comparison with normal activity levels could then be used to calculate the level of chemical exposure. The sensitivity of these types of sensors depends considerably on the chosen method of enzyme immobilization, transducer material employed, rate and number of chemical reaction(s), and sensitivity for a given electroactive species. Carbon nanotube detection of the single-step production of TCh, for example, was much better than the binary production of  $\text{H}_2\text{O}_2$  by  $\sim 60$ -fold. In both cases, use of a carbon nanotube electrode generated much greater S/N responses compared with an unmodified carbon screen-printed electrode, indicating a catalytic advantage. This advantage is attributed to the large surface area of the carbon nanotube available for redox reactions.

#### Applications of EC Immunosensors for Biomonitoring Metabolites or Protein Markers

Direct monitoring of key chemical or protein markers associated with a specific pesticide or disease offers the ability to quickly assess individuals. Competitive and sandwich-type EC immunoassays are being developed in our laboratories to provide the selectivity and sensitivity required for personalized biomonitoring. In addition, portable EC sensor platforms are being developed to integrate the EC sensor within an automated sample processor (Liu et al., 2005, 2006; Wu et al., 2007a,b; Liu et al. 2007b).

Two types of competitive binding EC immunoassays for the indirect detection of metabolite are being optimized using either an enzyme-tagged analog for detection of  $\text{H}_2\text{O}_2$  (Liu et al. 2005, 2006) or a QD-tagged analog for detection of acid hydrolyzed Cd ions (Wu et al., 2007a,b; Liu et al. 2007b).

A competitive EC immunoassay for the quantification of TCP, a metabolite marker for the insecticide chlorpyrifos, was recently developed (Liu et al., 2005, 2006). In this case, anti-TCP antibody was immobilized on magnetic particles to capture TCP, followed by the addition of sample and horseradish-peroxidase (HRP) enzyme-tagged TCP (analog), then addition of the HRP substrate 3,3',5,5'-tetramethylbenzidine dihydrochloride (TMB) to generate electroactive  $\text{H}_2\text{O}_2$  (Figure 7) (Liu et al., 2005). Using a sequential-injection analysis system to automatically deliver reagents and sample (Figure 4), antibody-coated magnetic beads (TCP-AB-MBs) were first pumped to a specific zone of the "reactor tube", where a magnetic field was applied to capture

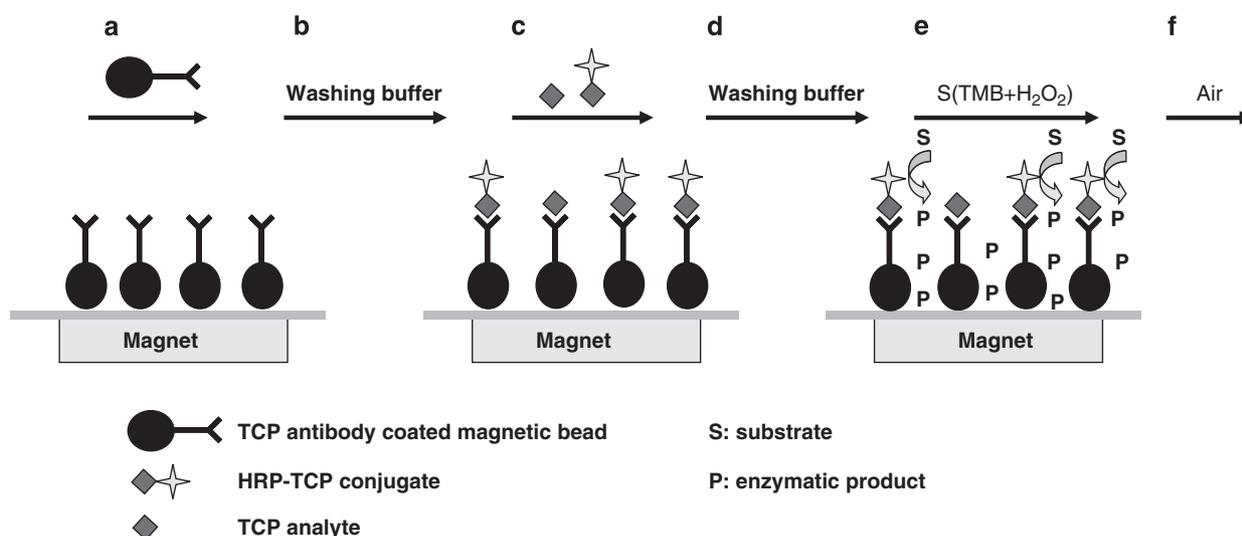

**Figure 7.** Diagram illustrating competitive immunoassay for 3,5,6-trichloro-2-pyridinol (TCP) determination. (a) immobilization of TCP antibody-coated magnetic beads to the internal wall of reactor tube by magnet; (b) washing beads with buffer; (c) injection of sample solution containing TCP analyte and TCP-horseradish peroxidase (TCP-HRP) for competitive immunoreaction; (d) washing beads with buffer; (e) injection of the substrate solution (TMB +  $\text{H}_2\text{O}_2$ ) to initiate enzymatic reaction; (f) analysis of enzymatic product by electrochemical measurement. Figure adapted from Liu et al. (2005) with permission.

the beads for further reactions. After an initial washing step, a premixed sample solution containing TCP and HRP-labeled TCP was introduced into the “reactor tube” containing the antibody-immobilized beads and incubated for ~20 min. Once the reaction was complete, the beads were washed again and the HRP substrate, TMB, was injected into the “reactor tube” to generate H<sub>2</sub>O<sub>2</sub>. Finally, the production of H<sub>2</sub>O<sub>2</sub> product was sent to a thin-layer flow cell for EC measurement (Figure 7). The reduction current required to reduce H<sub>2</sub>O<sub>2</sub> at the electrode surface is proportional to the amount of TCP present in the sample.

The selectivity of the TCP/HRP-TCP EC immunoassay was determined by using compounds structurally similar to TCP, including 2,4,5-trichlorophenol, 2,4-dichlorophenol, chlorpyrifos, chlorpyrifos-methyl, and trichlopyr. The results of these comparisons are presented in Table 1. For each insecticide, metabolite or structurally related chemical, a 50% inhibition concentration (IC<sub>50</sub>) was determined and compared with the TCP IC<sub>50</sub> and the extent of cross-reactivity (CR) was calculated (Liu et al., 2006). The structurally related compounds such as 2,4,5-trichlorophenol and 2,4-dichlorophenol demonstrated low cross reactivity ( $\leq 2\%$ ); whereas, the parent pesticides chlorpyrifos, chlorpyrifos-methyl, and trichlopyr showed little to no cross reactivity ( $<0.01\%$ ) (Liu et al., 2006). These results demonstrated that the TCP antibody coated magnetic beads were highly selective for TCP.

Performance of the sequential-injection analysis competitive EC immunoassay was optimized by adjusting reaction volumes and incubation times (Liu et al., 2005). Figure 8a shows the typical square-wave voltammogram responses with increasing TCP analyte concentrations. Well-defined peak shapes were used to calculate the concentration of the corresponding TCP in the sample matrix. The normalized signals, expressed as  $100(I/I_0)$  (where  $I$  and  $I_0$  are the reduction peak heights obtained with TCP standards and blank sample, respectively) were plotted *versus* TCP con-

centration. A sigmoidal-shaped calibration curve for TCP was used to calculate TCP in the sample (as is characteristic of a competitive immunoassay) (Figure 8b). The linear measuring range was 0.01–2.0  $\mu\text{g/l}$ , and the relative standard deviation was below 3.9% ( $n=6$ ). A detection limit was calculated from competitive curves as the analyte concentration for which the normalized signal was 90%. The detection limit was estimated to be ~6 ng/l.

To build in signal amplification and eliminate the need for enzyme-driven electroactive species, QDs can be used as tags along with the appropriate electrode sensor. For the competitive EC immunoassay, a QD can either be conjugated directly onto a metabolite (if the chemistry is appropriate) or conjugated to a chemically compatible structural analog, then used as the competitive analog. EC signal can then be generated by incubating the QD tag with acid (e.g., 1 M HCl) and detecting the hundreds to thousands of metal ions that dissolve from each QD.


Recently, we demonstrated the ultrasensitive detection and selection capability of QD-tagged sandwich immunoassays. Using commercially available monoclonal antibodies and QD conjugation kits (Invitrogen, Eugene, OR, USA), EC immunosensors were developed for ng/ml or pg/ml detection of interleukin-1 $\alpha$  (Figure 9) or prostate-specific antigen (Figure 10), respectively, in human plasma (Wu et al., 2007a,b; Liu et al., 2007a,b). For detection of interleukin-1 $\alpha$ , an immune and inflammatory response cytokine, primary interleukin-1 $\alpha$  antibody was bound to streptavidin-coated magnetic beads and QDs consisting of a CdSe core/ZnS coat were conjugated to secondary antibodies to sandwich the antigen, followed by acid hydrolysis (1 M HCl) of the QDs and detection of Cd<sup>2+</sup> ions with a bismuth/mercury coated screen-printed electrode using square-wave voltammetry (Figure 9). A detection limit of 18 pM (or 1.8 fmol) of cytokine could be detected in 200  $\mu\text{l}$  of sample with a linear range of 0.5–50 ng/ml. For detection of prostate specific antigen in human serum, a disposable EC immunosensors was manufactured containing separate zones for primary and secondary antigen capture (Figure 10). Primary monoclonal antibodies were conjugated with QDs and immobilized onto a glassy fiber pad and incubated with sample to capture the antigen, then the QD–antibody–antigen complex was migrated to a second zone containing immobilized secondary antibody for capture of tagged complex, followed by the addition of HCl at the second zone, solubilization of the QD and EC detection of Cd<sup>2+</sup> ions as the ions traversed laterally to the electrode surface hidden beneath a nitrocellulose membrane (Figures 10 and 11a). Prostate specific antigen could be detected down to 20  $\text{pg ml}^{-1}$  with 20 min of total incubation time. The EC assay was compared with results obtained from a commercially available ELISA prostate specific antigen kit (Alpha Diagnostics International) and similar concentration values were obtained for each assay but the reproducibility of the EC assay did vary more at lower

**Table 1.** Cross-reactivity of the bioelectrochemical magnetic immunoassay for various insecticide, their metabolites or structurally similar compounds.


Compound	IC <sub>50</sub> <sup>a</sup> (ng/ml)	CR <sup>b</sup> (%)
3,5,6-Trichloro-2-pyridinol (TCP)	0.45	100
2,4,5-Trichlorophenol	22	2.01
2,4-Dichlorophenol	430	0.11
<i>O,O</i> -Dimethyl- <i>O</i> -3,5,6-trichloro-2-pyridyl-phosphorothioate (chlorpyrifos-methyl)	$>1\text{E}^4$	$<0.01$
<i>O,O</i> -Diethyl- <i>O</i> -3,5,6-trichloro-2-pyridyl-phosphorothioate (chlorpyrifos)	$>1\text{E}^4$	$<0.01$
3,5,6-Trichloro-2-pyridyloxyacetic acid (trichlopyr)	$>1\text{E}^4$	$<0.01$

<sup>a</sup>Inhibition concentration estimated at 50%  $I/I_0$ .

<sup>b</sup>Percentage cross-reactivity  $\left(\frac{\text{IC}_{50}\text{TCP}}{\text{IC}_{50}\text{Similar}} \times 100\right)$

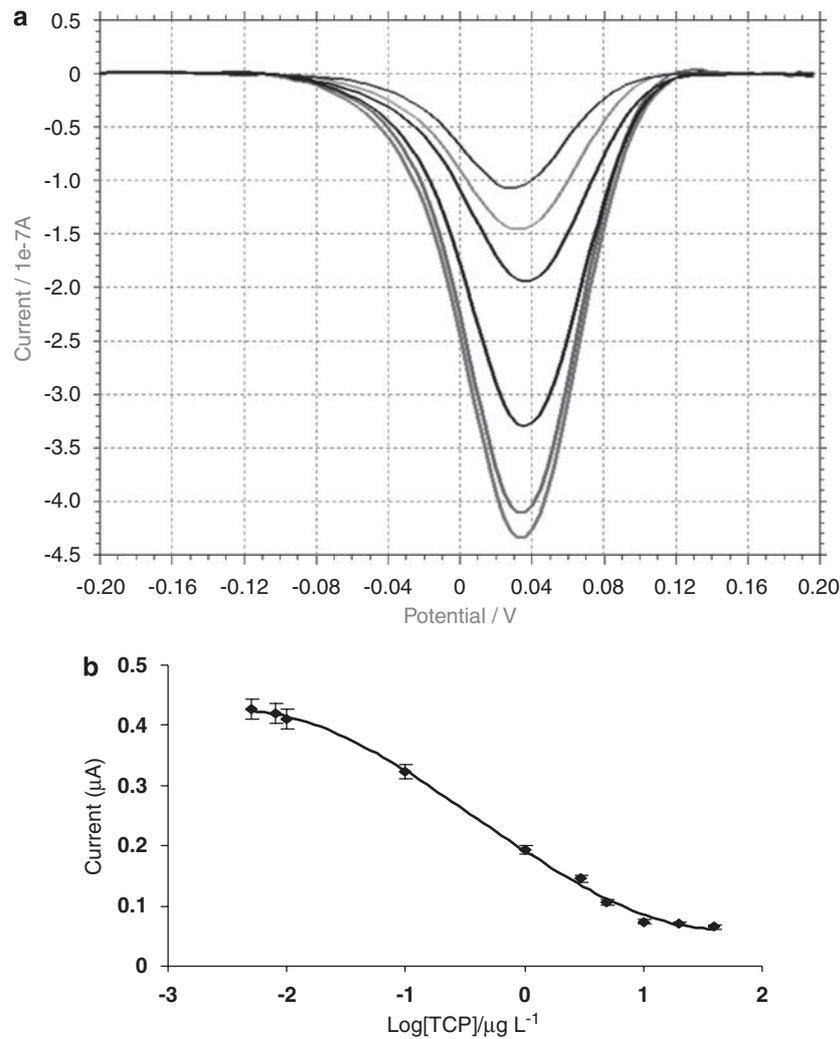


**Figure 8.** (a, top) Typical square-wave voltammetry of increasing TCP concentration in incubation solution. From bottom to top, the concentrations of TCP are 0, 0.005, 0.01, 0.05, 0.1, 0.5, 1, 2, 8, and 10 μg/l. (b, bottom) Sigmoidal calibration curve of TCP using 20 μl of TCP-Ab-MBs, 50 μl of TCP-HRP in 100 μl of sample solution, 100 μl of TMB-H<sub>2</sub>O<sub>2</sub> substrate solution, reaction time of 20 min. Figure adapted from Liu et al. (2005) with permission.

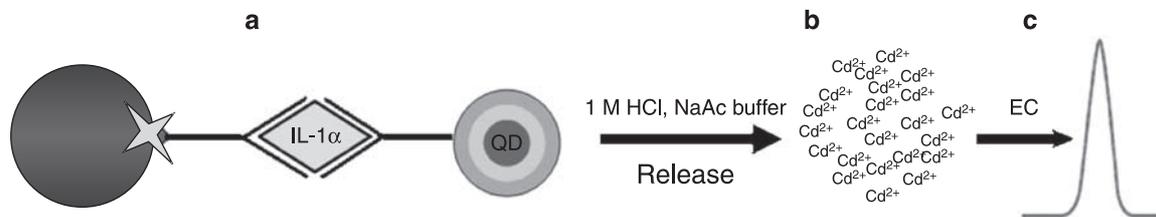

**Figure 9.** Solubilization and detection of quantum dot (QD) tags. Scheme of an EC sandwich immunoassay (a) using primary monoclonal anti-interleukin-1α antibody immobilized on magnetic bead and QD-tagged secondary anti-interleukin-1α antibody, followed by acid solubilization of CdSe core/ZnS coated QDs and detection of cadmium ions (b) by SWV (c). Adapted from Wu et al. (2007a,b) with permission.

concentrations; at 0.5 ng/ml the EC assay had a %CV of 24.5% whereas ELISA produced 7.1%, but at 2 ng/ml the EC assay had a 2.5% CV whereas ELISA produced 8.2%. These first set of experiments are quite promising and further optimizations and improvements are underway to enhance sample migration, analyte capture, and signal detection. In

addition, we have integrated the disposable EC immunoassay into a self-contained platform that can be interfaced with a computer containing the appropriate software (Figure 11b). Our focus is to develop low cost disposable immunochromatographic strips that can be rapidly evaluated in a fashion similar to glucose monitors used by diabetic patients.

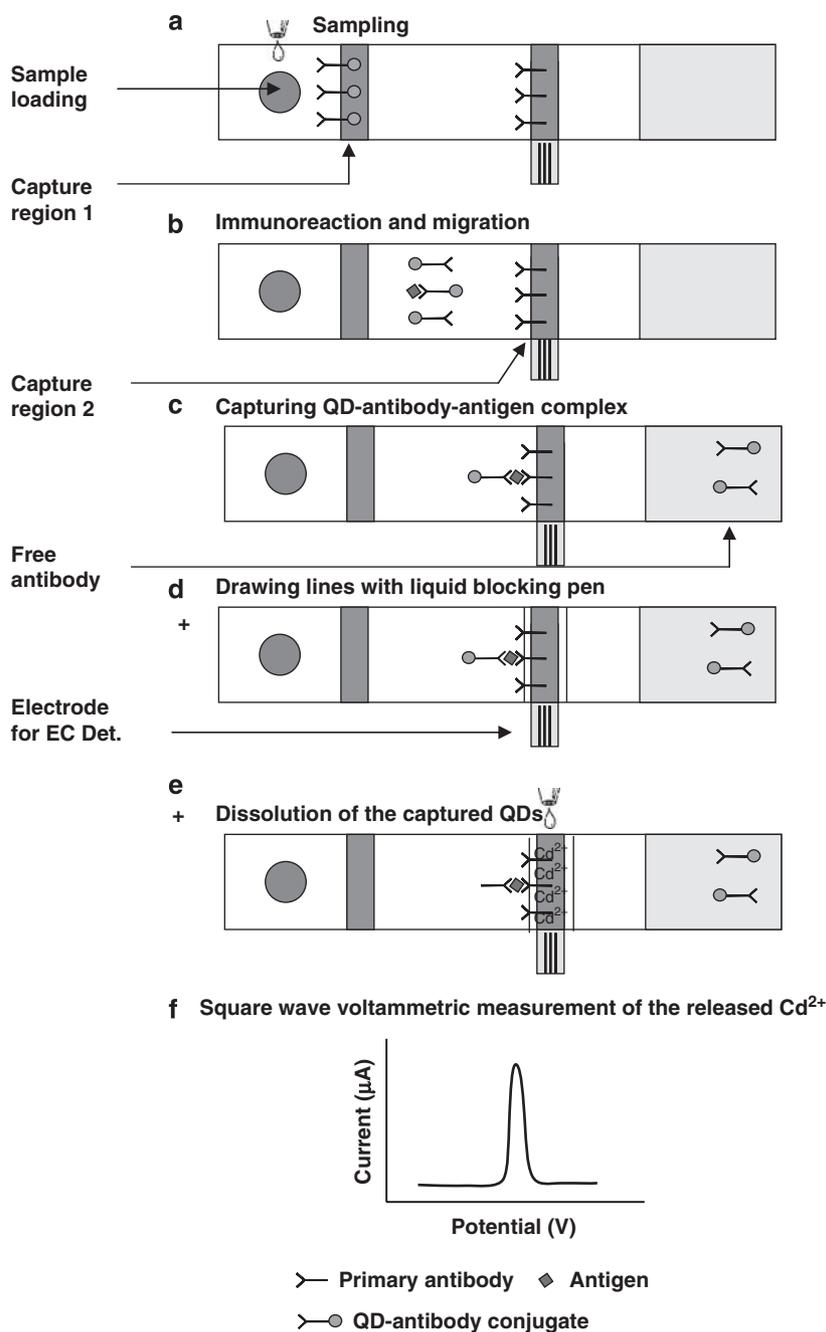


**Figure 10.** Development of a disposable EC sandwich immunoassay for the detection of prostate specific antigen, protein biomarkers of prostate cancer. Primary monoclonal antibodies were conjugated with QD and immobilized onto a glassy fiber pad and incubated with sample to capture the antigen (a), then the QD–antibody–antigen complex was migrated (b) to a second zone containing immobilized secondary antibody for capture of tagged antigen (c), followed by drawing two insulator lines with liquid blocker (super PAP pen, d) and the addition of HCl at the second zone, solubilization of the QD and EC detection of  $\text{Cd}^{2+}$  ions as the ions traversed laterally to the electrode surface hidden beneath a nitrocellulose membrane (e) to produce a square-wave voltammetry signal (f). Figure adapted from Liu et al. (2007a,b), with permission.


### Interpretation of Sensor Biomonitoring Results

An important consideration is whether the sensor platforms have adequate sensitivity to detect and quantify at environmentally relevant exposure concentrations. In this regard, computational dosimetry modeling has been used to establish

the sensitivity to detect TCP in saliva and blood of humans following repeated oral exposures to chlorpyrifos (Timchalk et al., 2007b). To accomplish this, a physiologically based pharmacokinetic and pharmacodynamic model was used to simulate dosimetry and dynamic response in humans (Timchalk et al., 2002). The model simulated repeated

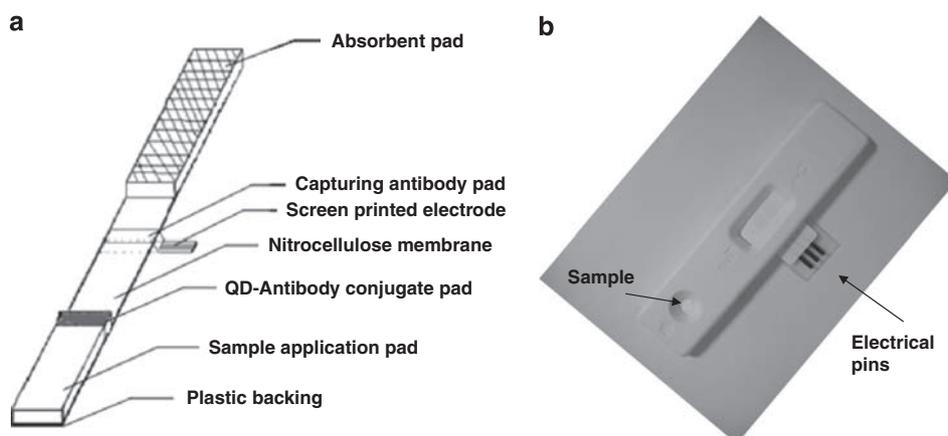

**Figure 11.** (a) Schematic of a disposable EC immunosensors containing a primary capture region using an immobilized QD-tagged antiprostase antigen antibody, a secondary capture regions containing secondary antibodies. Upon treatment with 1 M HCl at the secondary region, cadmium ions are released and electrophoretically migrate to a bismuth/mercury-coated screen-printed electrode beneath a nitrocellulose membrane. (b) Sample is added to the strip and the electrical pins of the strip are inserted into an electronic control box of the portable EC platform. Voltage is applied to the strip and the signal output is displayed on a PC. Figure is adapted from Liu et al. (2007a,b) with permission.

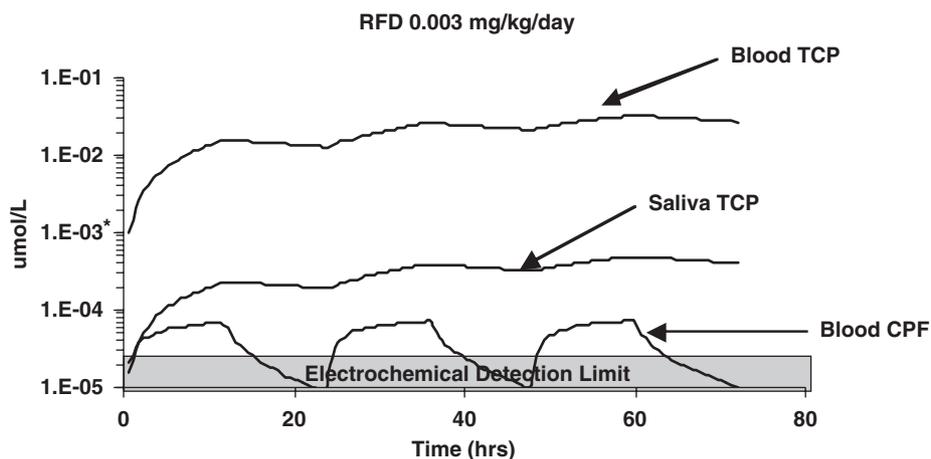

**Figure 12.** Computational pharmacokinetic model simulation of 3,5,6-trichloro-2-pyridinol (TCP) in blood and saliva and chlorpyrifos in blood following a repeated (3-day) dietary exposure (12 h/day) to 0.003 mg/kg/day (RfD). The detection limit (\*) for the ELISA assay is based on the value reported by the manufacturer of the TCP rapid Assay<sup>®</sup> kit (0.25  $\mu\text{g/l}$  or  $1\text{E}^{-3}$   $\mu\text{mol/l}$ ). Figure adapted from Timchalk et al. (2007a,b) with permission.

dietary exposure to chlorpyrifos over a 72 h period at the established EPA Reference Dose (RfD) of 0.003 mg/kg/day (EPA, 1994). The results from these simulations and the reported detection limits for a commercial TCP ELISA and the EC immunoassay are presented in Figure 12. These simulations suggest that the EC immunoassay theoretically has the needed sensitivity to detect TCP in both blood and saliva based upon the anticipated range of concentrations at the RfD level. Future *in vivo* studies are needed to substantiate the model simulations and validate the detection limits for the sensor platforms.

Although biomonitoring offers one of the best approaches for accurately assessing human dosimetry and for determining risk from both occupational and environmental exposure

to xenobiotics (Friberg and Elinder, 1993; Christensen, 1995) the ability to better interpret the results of biomonitoring is also needed (Hays et al., 2007). One potentially useful approach is to use “reverse dosimetry” to back-extrapolate a population-based distribution of biomonitoring data to a distribution of exposure doses (Hays et al., 2007). In this regard, Tan et al. (2007) recently used a “reverse dosimetry” approach to integrate outputs from physiologically based pharmacokinetic modeling, exposure characterizations, and Monte Carlo and statistical analyses to estimate the distribution of exposures to trihalomethanes which could then be compared with animal-based health standards (i.e., RfD). With regard to the organophosphate insecticide chlorpyrifos a similar approach was used based on a simple

pharmacokinetic model of TCP urinary excretion kinetics to estimate dosimetry in children (Rigas et al., 2001). In this particular study, however, the reverse pharmacokinetic modeling of urinary TCP generally over predicted dose. As suggested by Rigas et al. (2001) and others, exposure to organophosphate breakdown products such as TCP as residues on food or in the environment could contribute to the greater than expected amounts of TCP in urine (Wilson et al. 2003; Lu et al., 2005; Morgan et al., 2005; Timchalk et al., 2007b). One way to strengthen predictive assessments would be to develop computational dosimetry models based on metabolic endpoints and multiple biomarkers (e.g., for pesticide exposures: cholinesterase inhibition, metabolites, and protein biomarkers).

## Discussion

### *Summary Considerations for EC Sensors and Future Opportunities*

Disposable EC sensors offer a wide-range of applications for analysis of chemical compounds within biological systems, given they are minimally susceptible to matrix effects and are selective for the compound of interest. An important consideration for sensor development is the optimization of the sensor performance in a broad range of biological matrices (i.e., blood, urine, saliva) that are routinely used to biological monitoring (Yantasee et al., 2007a). Specifically, the EC sensor must be validated for analytical performance and cross-validated with well-established analytical methods, such as mass spectrometry and ELISA. Characteristics such as accuracy, precision, sensitivity, selectivity, repeatability, and stability should be addressed. Second, a robust evaluation is needed to assess the potential for detection interference using biological matrices. Third, *in vivo* animal and *in vitro* human validation studies are needed to assess the selectivity, sensitivity, and robustness of the sensor platforms. And finally, appropriate field evaluation studies are needed to ascertain the performance of the sensor platforms under a broad range of robust conditions that exist in the “real-world”.

Future opportunities exist to investigate the use of alternative affinity or sequestration stationary phases, such as titanium oxide, zirconium oxide, aptamers (small nucleic acids strands), chelators, self-assembled monolayers, polymer-modified nanoparticles, and nanostructured hydrogels (Flounders et al., 1999; Singh et al., 1999; Liu and Lin, 2005; Mattigod et al., 2005; Nayak and Lyon, 2005; Castellana et al., 2006; Yantasee 2007b; Li and Ho, 2008; Li et al., 2008; Xiao and Li, 2008). In addition, throughput could be extended by developing multichannel, parallel, and multiplexed detection of multiple analytes (Tang et al., 2002; Dong et al., 2007; Polsky et al., 2008).

## Conclusion

We are all routinely exposed to a broad range of chemicals that are present within the environment; including pollutants within the air we breathe, the food we eat, and the water we drink. Exposure to these chemicals may be associated with our home or work environments, as part of our jobs, or as lifestyle choices. Epidemiology studies have been utilized to ascertain an association between environmental chemical exposures and human disease. As recently noted, current epidemiology study designs are seriously hampered due to the inability to make definitive associations between chemical exposures and disease (Weis et al., 2005). Biomonitoring studies that can routinely measure chemical and biological molecular markers of exposure and the development of dosimetry models that can factor in these markers offers the potential to better understand the risk factors associated with adverse health. Inexpensive, sensitive, flexible, and portable biomonitoring tools need to be developed that can handle the logistics of monitoring the myriad of markers associated with chemical exposures among different populations. The development of portable nanotechnology-based EC sensors has the potential to meet the needs for low cost, rapid, high-throughput, and ultrasensitive bioassays for biomonitoring an array of chemical markers. Highly selective EC sensors capable of pM sensitivity, high-throughput (3600 samples per h) with low sample requirements (<50  $\mu$ l) have already been demonstrated; and improved EC sensors are on the horizon. To advance the utility and improve the quality of these sensors for risk assessment and epidemiological studies, it would be ideal to form close collaborations between chemists, toxicologists, and epidemiologists.

## Acknowledgements

This work was performed at Pacific Northwest National Laboratory (PNNL) supported partially by grant number NS058161-01 from the National Institutes of Health CounterACT Program through the National Institute of Neurological Disorders and Stroke, partially by CDC/NIOSH Grant R01 OH008173, and partially by grant number U54 ES16015 from the National Institute of Environmental Health Sciences (NIEHS), NIH. The contents of this publication are solely the responsibility of the authors and do not necessarily represent the official views of the Federal Government. The research described in this paper was partly performed at the Environmental Molecular Sciences Laboratory, a national scientific user facility sponsored by the DOE's Office of Biological and Environmental Research and located at PNNL. PNNL is operated by Battelle for DOE under Contract DE-AC05-76RL01830.

## References

- Al-Saleh I.A. Pesticides: a review article. *J Environ Path Toxicol Oncol* 1994; 13: 151–161.
- Andrescu S., and Marty J.-L. Twenty years research in cholinesterase biosensors: from basic research to practical applications. *Biomol Eng* 2006; 23: 1–15.
- Angerer J., Bird M.G., Burke T.A., Doerrer N.G., Needham L., Robison SH, et al. Strategic biomonitoring initiatives: moving the science forward. *Toxicol Sci* 2006; 93(1): 3–10.
- Arnold E.K., and Beasley V.R. The pharmacokinetics of chlorinated phenoxy acid herbicides: a literature review. *Vet Hum Toxicol* 1989; 31(2): 121–125.
- Ashley K. Developments in electrochemical sensors for occupational and environmental health applications. *J Hazard Mater* 2003; 102: 1–12.
- Aspelin A.L. *Pesticide Industry Sales and Usage: 1990 and 1991 Market Estimates*. Office of Pesticide Programs, US Environmental Protection Agency, EPA, Washington, DC, 1992, 733-K-92-001.
- Aspelin A.L. *Pesticide Industry Sales and Usage: 1992 and 1993 Market Estimates*. Office of Pesticide Programs, US Environmental Protection Agency, EPA, Washington, DC, 1994, 733-K-94-001.
- Authier L., Grossiord C., Brossier P., and Limoges B. Gold nanoparticle-based quantitative electrochemical detection of amplified human cytomegalovirus DNA using disposable microband electrodes. *Anal Chem* 2001; 73: 4450–4456.
- Badihi-Mossberg M., Buchner V., and Rishpon J. Electrochemical biosensors for pollutants in the environment. *Electroanalysis* 2007; 19: 2015–2028.
- Bard A.J., and Faulkner L.R. *Electrochemical Methods: Fundamentals and Applications*. John Wiley and Sons Inc., New York, 1980, pp 413–414.
- Barr D.B., Bravo R., Weerasekera G., Caltabiano L.M., Whitehead Jr R.D., et al. Concentrations of dialkyl phosphate metabolites of organophosphorus pesticides in the U.S. population. *Environ Health Perspect* 2004; 112: 186–200.
- Belmont C., Tercier M.L., Buffle J., Fiaccabrinno G.C., and Koudelka-Hep M. Mercury-plated iridium-based microelectrode array for trace metals detection by voltammetry: optimum conditions and reliability. *Anal Chim Acta* 1996; 329: 203–214.
- Berkowitz G.S., Wetmur J.G., Birman-Deych E., Obel J., Lapinski R.H., et al. In utero pesticide exposure, maternal paraoxonase activity, and head circumference. *Environ Health Perspect* 2004; 112(3): 388–391.
- Black R.M., Harrison J.M., and Read R.W. The interaction of sarin and soman with plasma proteins: the identification of a novel phosphorylation site. *Arch Toxicol* 1999; 73: 123–126.
- Borzelleca J.F., and Skalsky H.L. The excretion of pesticides in saliva and its value in assessing exposure. *J Environ Sci Health* 1980; B15(6): 843–866.
- Boter H.L., and Ooms A.J.J. Stereospecificity of hydrolytic enzymes in their reaction with optically active organophosphorus compounds. II. The inhibition of aliesterase, acetylcholinesterase, chymotrypsin and trypsin by *S*-alkyl *para*-nitrophenyl methylphosphonothiolates. *Biochem Pharmacol* 1967; 16: 1563–1569.
- Bradman A., Eskenazi B., Barr D., Bravo R., Castorina R., et al. Organophosphate urinary metabolite levels during pregnancy and after delivery in women living in an agricultural community. *Environ Health Perspect* 2005; 112(11): 1802–1807.
- Castellana E.T., Kataoka S., Albertorio F., and Cremer P.S. Direct writing of metal nanoparticle films inside sealed microfluidic channels. *Anal Chem* 2006; 78: 107–112.
- CDC. *Centers for Disease Control and Prevention. Third National Report on Human Exposure to Environmental Chemicals*. Department of Health and Human Services, NCEH Pub. No. 05-0570 2005.
- Chambers J.E., and Chambers H.W. Oxidative desulfation of chlorpyrifos, chlorpyrifos-methyl, and leptophos by rat brain and liver. *J Biochem Toxicol* 1989; 4(1): 201–203.
- Chen G., Lin Y.H., and Wang J. Monitoring environmental pollutants by microchip capillary electrophoresis with electrochemical detection. *Talanta* 2006a; 68: 497–503.
- Chen S.H., Yuan R., Chai Y.Q., Zhang L.Y., Wang N., and Li X.L. Amperometric third-generation hydrogen peroxide biosensor based on the immobilization of hemoglobin on multiwall carbon nanotubes and gold colloidal nanoparticles. *Biosens Bioelectron* 2007; 22: 1268–1274.
- Chester G. Evaluation of agricultural worker exposure to and absorption of pesticides. *Occup Hyg* 1993; 37: 509–523.
- Christensen J.M. Human exposure to toxic metals: factors influencing interpretation of biomonitoring results. *Sci Total Environ* 1995; 166: 89–135.
- Collins G.E., and Lu Q. Microfabricated capillary electrophoresis sensor for uranium (VI). *Anal Chim Acta* 2001; 436: 181–189.
- Cui R., Pan H.C., Zhu J.J., and Chen H.Y. Versatile immunosensor using CdTe quantum dots as electrochemical and fluorescent labels. *Anal Chem* 2007; 79: 8494–8501.
- Dabek-Zlotorzynska E., Chen H., and Ding L.Y. Recent advances in capillary electrophoresis and capillary electrochromatography of pollutants. *Electrophoresis* 2003; 24: 4128–4149.
- Drummond T.G., Hill M.G., and Barton J.K. Electrochemical DNA sensors. *Nat Biotechnol* 2003; 21(10): 1192–1199.
- Dong H., Li C.M., Zhang Y.F., Cao X.D., and Gan Y. Screen-printed microfluidic device for electrochemical immunoassay. *Lab Chip* 2007; 7(12): 1752–1758.
- Du D., Ding J.W., Cai J., and Zhang A.D. One-step electrochemically deposited interface of chitosan-gold nanoparticles for acetylcholinesterase biosensor design. *J Electroanal Chem* 2007; 605: 53–60.
- Ecobichon D.J., and Comeau A.M. Pseudocholesterases of mammalian plasma: physicochemical properties and organophosphate inhibition in eleven species. *Toxicol Appl Pharmacol* 1973; 24(1): 92–100.
- Ecobichon D.J. Toxic effects of pesticides. In: Klassen C.D. (Ed.). *Casarett & Doull's Toxicology The Basic Science of Poisons*, 6th edn. McGraw-Hill, New York, 2001, pp. 763–810.
- Elhanany E., Ordentlich A., Dgany O., Kaplan D., Segall Y., et al. Resolving pathways of interaction of covalent inhibitors with the active site of acetylcholinesterases: MALDI-TOS/MS analysis of various nerve agent phosphyl adducts. *Chem Res Toxicol* 2001; 14: 912–918.
- EPA. U.S. Environmental Protection Agency, Integrated Risk Information System Database, Washington DC, 1994, 5–54.
- Eskenazi B., Harley K., Bradman A., Weltzien E., Jewell N.P., et al. Association of in utero organophosphate pesticide exposure and fetal growth and length of gestation in an agricultural population. *Environ Health Perspect* 2004; 112(10): 1116–1124.
- Flounders A.W., Singh A.K., Volponi J.V., Carichner S.C., Wally K., Simonian A.S., et al. Development of sensors for direct detection of organophosphates. Part II: sol-gel modified field effect transistor with immobilized organophosphate hydrolase. *Biosens Bioelectron* 1999; 14: 715–722.
- Fonnum F., Sterri S.H., Aas P., and Johnsen H. Carboxylesterase, importance for detoxification of organophosphorus anticholinesterases and trichothecenes. *Fundam Appl Toxicol* 1985; 5: S29–S38.
- Friberg L., and Elinder C.G. Biological monitoring of toxic metals. *Scand J Work Environ Health* 1993; 19(Suppl 1): 7–13.
- Galve R., Nickkova M., Camps F., Sanchez-Baeza F., and Marco M.P. Development and evaluation of an immunoassay for biological monitoring chlorophenols in urine as potential indicators of occupational exposure. *Anal Chem* 2002; 74(2): 468–478.
- Gil F., and Pla A. Biomarkers as biological indicators of xenobiotic exposure. *J Appl Toxicol* 2001; 21: 245–255.
- Gilbert D.M., and Sale T.C. Sequential electrolytic oxidation and reduction of aqueous phase energetic compounds. *Environ Sci Technol* 2005; 39: 9270–9277.
- Guerrieri A., and Palmisano F. An Acetylcholinesterase/choline oxidase-based amperometric biosensor as a liquid chromatography detector for acetylcholine and choline determination in brain tissue. *Anal Chem* 2001; 73: 2875–2882.
- Guo S.J., and Wang E.K. Synthesis and electrochemical applications of gold nanoparticles. *Anal Chim Acta* 2007; 598: 181–192.
- Hainfeld J.F., and Powell R.D. New frontiers in gold labeling. *J Histochem Cytochem* 2000; 48: 471–480.
- Haláček J., Hepel M., and Skladal P. Investigation of highly sensitive piezoelectric immunosensors for 2,4-dichlorophenoxyacetic acid. *Biosens Bioelectron* 2001; 16(4–5): 253–260.
- Hanrahan G., Patil D.G., and Wang J. Electrochemical sensors for environmental monitoring: design, development and applications. *J Environ Monit* 2004; 6: 657–664.
- Hardt J., and Angerer J. Determination of dialkyl phosphates in human urine using gas chromatography–mass spectrometry. *J Anal Toxicol* 2000; 8(24): 678–684.
- Hays S.M., Becker R.A., Leung H.W., Aylward L.L., and Pyatt D.W. Biomonitoring equivalents: a screening approach for interpreting biomonitoring results from a public health risk perspective. *Reg Toxicol Pharmacol* 2007; 47: 96–109.

- He L., and Toh C.S. Recent advances in Anal Chem—a material approach. *Anal Chim Acta* 2006; 556: 1–15.
- Henn B.C., McMaster S., and Padilla S. Measuring cholinesterase in human saliva. *J Toxicol Environ Health A* 2006; 69: 1805–1818.
- Jain K.K. Applications of nanobiotechnology in clinical diagnostics. *Clin Chem* 2007; 53: 2002–2009.
- Johnson M.K., and Glynn P. Neuropathy target esterase (NTE) and organophosphorus-induced delayed polyneuropathy (OPIDP): recent advances. *Toxicol Lett* 1995; 82–83: 459–463.
- Johnson M.K. Organophosphorus esters causing delayed neurotoxic effects—mechanism of action and structure/activity studies. *Arch Toxicol* 1975; 34: 259–288.
- Kim S.N., Rusling J.F., and Papadimitrakopoulos F. Carbon nanotubes for electronic and electrochemical detection of biomolecules. *Adv Mater* 2007; 19: 3214–3228.
- Knecht E., Martinez-Ramon A., and Grisolia S. Electron microscopic localization of glutamate dehydrogenase in rat liver mitochondria by an immunogold procedure and monoclonal and polyclonal antibodies. *J Histochem Cytochem* 1986; 34: 912–922.
- Kousba A.A., Poet T.S., and Timchalk C. Characterization of the *in vitro* kinetic interaction of chlorpyrifos-oxon with rat saliva cholinesterase: a potential biomonitoring matrix. *Toxicology* 2003; 188: 219–232.
- Kröger S., Setford S.J., and Turner A.P. Immunosensor for 2,4-dichlorophenoxyacetic acid in aqueous/organic solvent soil extracts. *Anal Chem* 1998; 70(23): 5047–5053.
- Li B., Schopfer L.M., Hinrichs S.H., Masson P., and Lockridge O. Matrix-assisted laser desorption/ionization time-of-flight mass spectrometry assay for organophosphorus toxicants bound to human albumin at Tyr411. *Anal Biochem* 2007; 361: 263–272.
- Li B., Wang Y., and Dong S. Amplified electrochemical aptasensor taking AuNPs based sandwich sensing platform as a model. *Biosens Bioelectron* 2008; 23(7): 965–970.
- Li N., and Ho C.-M. Aptamer-based optical probes with separated molecular recognition and signal transduction modules. *J Am Chem Soc* 2008; 130(8): 2380–2381.
- Lin Y.H., Lu F., and Wang J. Disposable carbon nanotube modified screen-printed biosensor for amperometric detection of organophosphorus pesticides and nerve agents. *Electroanalysis* 2004; 16: 145–149.
- Lin Y.H., Yantasee W., and Wang J. Carbon nanotubes CNTs for the development of electrochemical biosensors. *Front Biosci* 2005; 10: 492–505.
- Lin Y.Y., Liu G.D., Wai C.M., and Lin Y.H. Magnetic beads-based bioelectrochemical immunoassay of polycyclic aromatic hydrocarbons. *Electrochem Commun* 2007; 9: 1547–1552.
- Liu G.D., Riechers S.L., Timchalk C., and Lin Y. Sequential injection/electrochemical immunoassay for quantifying the pesticide metabolite 3,5,6-trichloro-2-pyridinol. *Electrochem Commun* 2005; 7: 1463–1470.
- Liu G.D., and Lin Y.H. Electrochemical sensor for organophosphate pesticides and nerve agents using zirconia nanoparticles as selective sorbents. *Anal Chem* 2005; 77: 5894–5901.
- Liu G., Timchalk C., and Lin Y. Bioelectrochemical magnetic immunosensing of trichloropyridinol: a potential insecticide biomarker. *Electroanalysis* 2006; 18(16): 1605–1613.
- Liu G., and Lin Y. Biosensor based on self-assembling acetylcholinesterase on carbon nanotubes for flow injection/amperometric detection of organophosphate pesticides and nerve agents. *Anal Chem* 2006; 78: 835–843.
- Liu G., Wang J., Wu H., Lin Y.-Y., and Lin Y. Nanovehicles based bioassay labels. *Electroanalysis* 2007a; 19: 777–785.
- Liu G., Lin Y.-Y., Wang J., Wu H., Chien M.W., and Lin Y. Disposable electrochemical immunosensor diagnosis device based nanoparticle probe and immunochromatographic strip. *Anal Chem* 2007b; 79: 7644–7653.
- Liu J., and Lu Y. A colorimetric lead biosensor using DNAzyme-directed assembly of gold nanoparticles. *J Am Chem Soc* 2003; 125: 6642–6643.
- Lu C., Bravo R., Caltabiano L.M., Irish R.M., Weerasekera G., et al. The presence of dialkylphosphate in fresh fruit juices: implication for organophosphorus pesticide exposure and risk assessments. *J Toxicol Environ Health A* 2005; 68: 209–227.
- Ma T., and Chambers J.E. Kinetic parameters of desulfuration and dearylation of parathion and chlorpyrifos by rat liver microsomes. *Food Chem Toxicol* 1994; 32(8): 763–767.
- Manz A., Fetting J.C., Verpoorte E., Ludi H., Widmer H.M., and Harrison D.J. Micromachining of monocrystalline silicon and glass for chemical analysis systems. *Trends Anal Chem* 1991; 10: 144–149.
- Mattigod S.V., Fryxell G.E., Alford K., Gilmore T., Parker K., et al. Functionalized TiO<sub>2</sub> nanoparticles for use *in situ* anion immobilization. *Environ Sci Technol* 2005; 39(18): 7306–7310.
- Merkoci A., Aldavert M., Tarrason G., Eritja R., and Alegret S. Toward and ICPMS-linked DNA assay based on gold nanoparticles immunocrosslinked through peptide sequences. *Anal Chem* 2005; 77: 6500–6503.
- Morgan M.K., Sheldon L.S., Croghan C.W., Jones P.A., Robertson G.L., et al. Exposures of preschool children to chlorpyrifos and its degradation product 3,5,6-trichloro-2-pyridinol in their everyday environment. *J Exp Anal Environ Epidemiol* 2005; 15: 297–309.
- Nayak S., and Lyon L.A. Soft nanotechnology and soft nanoparticles. *Angew Chem Int Ed* 2005; 44: 7686–7708.
- Neufeld T., Eshkenazi I., Cohen E., and Rishpon J. A micro flow injection electrochemical biosensor for organophosphorus pesticides. *Biosens Bioelectron* 2000; 15: 323–329.
- Nolan R.J., Rick D.L., Freshour N.L., and Saunders J.H. Chlorpyrifos: pharmacokinetics in human volunteers. *Toxicol Appl Pharmacol* 1984; 73: 8–15.
- Ooms A.J.J., and van Dijk C. The reaction of organophosphorus compounds with hydrolytic enzymes-III: the inhibition of chymotrypsin and trypsin. *Biochem Pharmacol* 1966; 15: 1361–1377.
- Patolsky F., Zheng G.F., and Lieber C.M. Fabrication of silicon nanowire devices for ultrasensitive, label-free, real-time detection of biological and chemical species. *Nat Protoc* 2006; 1: 1711–1724.
- Peebles E.S., Schopfer L.M., Duysen E.G., Spaulding R., Voelker T., et al. Albumin a new biomarker for organophosphorus toxicant exposure, identified by mass spectrometry. *Toxicol Sci* 2005; 83: 303–312.
- Peoples S.A., and Knaak J. Monitoring pesticide blood cholinesterase and analyzing blood and urine for pesticides and their metabolites. In: Plimmer J.R. (Ed.). *Pesticide Residues and Exposure*, Am Chem Soc Symp Series No. 182. American Chemical Society, Washington, DC, 1982, pp. 41–57.
- Piras L., and Reho S. Colloidal gold based electrochemical immunoassays for the diagnosis of acute myocardial infarction. *Sens Actuators B* 2005; 111–112: 450–454.
- Polhuijs M., Langenberg J.P., and Benschop H.P. New method for retrospective detection of exposure to organophosphorus anticholinesterases: application to alleged sarin victims of Japanese terrorists. *Toxicol Appl Pharmacol* 1997; 146: 156–161.
- Pumera M., Sanchez S., Ichinose I., and Tang J. Electrochemical nanobiosensors. *Sens Actuators B Chem* 2007; 123: 1195–1205.
- Rigas M.L., Okino M.S., and Quackenboss J.J. Use of a pharmacokinetic model to assess chlorpyrifos exposure and dose in children, based on urinary biomarker measurements. *Toxicol Sci* 2001; 61: 374–381.
- Renedo O.D., Alonso-Lomillo M.A., and Martinez M.J.A. Recent developments in the field of screen-printed electrodes and their related applications. *Talanta* 2007; 73: 202–219.
- Ryhanen R.J. Pseudocholinesterase activity in some human body fluids. *Gen Pharmacol* 1983; 14(4): 459–460.
- Sadik O.A., and Van Emon J.M. Applications of electrochemical immunosensors to environmental monitoring. *Biosens Bioelectron* 1996; 11(8): 1–9.
- Savolainen K. Understanding the toxic actions of organophosphates. In: Krieger R.I. (Ed.). *Handbook of Pesticide Toxicology*, Vol. 2 Academic Press, San Diego, 2001, pp. 1013–1041.
- Singh A.K., Flounders A.W., Volponi J.V., Ashley C.S., Wally K., and Schoeninger J.S. Development of sensors for direct detection of organophosphates. Part I: immobilization, characterization and stabilization of acetylcholinesterase and organophosphate hydrolase on silica supports. *Biosens Bioelectron* 1999; 14: 703–713.
- Skoog D.A., and Leary J.J. *Principles of Instrumental Analysis*, 4th edn. Harcourt Brace College Publishers, New York, 1992, pp. 535–564.
- Sole S., and Alegret S. Environmental toxicity monitoring using electrochemical biosensing systems. *Environ Sci Pollut Res Int* 2001; 8: 256–264.
- Tan Y.M., Liao K.H., and Clewell III H.J. Reverse dosimetry: interpreting trihalomethanes biomonitoring data using physiologically based pharmacokinetic modeling. *J Expo Sci Environ Epidemiol* 2007; 17(7): 591–603.
- Tang T.-C., Deng A., and Huang H.-J. Immunoassay with microtiter plate incorporated multichannel electrochemical detection system. *Anal Chem* 2002; 74: 2617–2621.
- Tansil N.C., and Gao Z.Q. Nanoparticles in biomolecular detection. *Nano Today* 2006; 1: 28–37.

- Tasis D., Tagmatarchis N., Bianco A., and Prato M. Chemistry of carbon nanotubes. *Chem Rev* 2006; 106: 1105–1136.
- Timchalk C. Comparative inter-species pharmacokinetics of phenoxyacetic acid herbicides and related organic acids. Evidence that the dog is not a relevant species for evaluation of human health risk. *Toxicology* 2004; 200: 1–19.
- Timchalk C., Busby A., Campbell J.A., Needham L.L., and Barr D.B. Comparative pharmacokinetics of the organophosphorus insecticide chlorpyrifos and its major metabolites diethylphosphate, diethylthiophosphate and 3,5,6-trichloro-2-pyridinol in the rat. *Toxicology* 2007b; 237: 145–157.
- Timchalk C., Campbell J.A., Liu G., Lin Y., and Kousba A.A. Development of a non-invasive biomonitoring approach to determine exposure to the organophosphorus insecticide chlorpyrifos in rat saliva. *Toxicol Appl Pharmacol* 2007a; 219: 217–225.
- Timchalk C., Nolan R.J., Mendrala A.L., Dittenber D.A., Brzak K.A., and Mattsson J.L. A physiologically based pharmacokinetic and pharmacodynamic (PBPK/PD) model for the organophosphate insecticide chlorpyrifos in rats and humans. *Toxicol Sci* 2002; 66: 34–53.
- Timchalk C., Poet T., Kousba A., Campbell J., and Lin Y. Noninvasive biomonitoring approaches to determine dosimetry and risk following acute chemical exposure: analysis of lead or organophosphate insecticide in saliva. *J Toxicol Environ Health A* 2004; 67: 635–650.
- Timchalk C., Poet T.S., Lin Y., Weitz K.K., Zhao R., et al. Development of an integrated microanalytical system for analysis of lead in saliva and linkage to a physiologically based pharmacokinetic model describing lead saliva secretion. *AHHAJ* 2001; 62: 295–302.
- Trojanowicz M. Analytical applications of carbon nanotubes: a review. *Trac-Trends Anal Chem* 2006; 25: 480–489.
- Velasco-Arjona A., Manclús J.J., Montoya A., and Luque de Castro M.D. Robotic sample pretreatment-immunoassay determination of chlorpyrifos metabolite (TCP) in soil and fruit. *Talanta* 1997; 45: 371–377.
- Wang J. Nanoparticle-based electrochemical bioassays of proteins. *Electroanalysis* 2007; 19: 769–776.
- Wang J., Chatrathi M.P., Mulchandani A., and Chen W. Capillary electrophoresis microchips for separation and detection of organophosphate nerve agents. *Anal Chem* 2001; 73: 1804–1808.
- Wang J., Li J.H., Baca A.J., Hu J.B., Zhou F.M., Yan W., and Pang D.W. Amplified voltammetric detection of DNA hybridization via oxidation of ferrocene caps on gold nanoparticle/streptavidin conjugates. *Anal Chem* 2003; 75: 3941–3945.
- Wang J., and Li R. On-valve electrochemical detector for high-speed flow injection analysis. *Anal Chem* 1990; 62: 2414–2416.
- Wang J., Liu G.D., Engelhard M.H., and Lin Y.H. Sensitive immunoassay of a biomarker tumor necrosis factor-alpha based on polyguanine-functionalized silica nanoparticle label. *Anal Chem* 2006a; 78: 6974–6979.
- Wang J., Liu G.D., and Lin Y.H. Amperometric choline biosensor fabricated through electrostatic assembly of bienzyme/polyelectrolyte hybrid layers on carbon nanotubes. *Analyst* 2006b; 131: 477–483.
- Wang J., Liu G.D., Timchalk C., and Lin Y. Carbon nanotube-based electrochemical sensor for assay of salivary cholinesterase enzyme activity: an exposure biomarker of organophosphate pesticides and nerve agents. *Environ Sci Technol* 2008a; 42: 2688–2693.
- Wang J., Liu G.D., Wu H., and Lin Y.H. Quantum dot-based electrochemical immunosensor for high throughput screening of prostate-specific antigen. *Small* 2008b; 4: 82–86.
- Wang J., Liu G.D., Wu H., and Lin Y.H. Sensitive electrochemical immunoassay for 2, 4, 6-trinitrotoluene based on functionalized silica nanoparticle labels. *Anal Chim Acta* 2008c; 610(1): 112–118.
- Wang J., Pumera M., Chatrathi M.P., Escarpa A., Musameh M., Collins G., Mulchandani A., Lin Y., and Olsen K. Single-channel microchip for fast screening and detailed identification of nitroaromatic explosives or organophosphate nerve agents. *Anal Chem* 2002; 74: 1187–1191.
- Weis B.K., Balshaw D., Barr J.R., Brown D., Ellisman M., Lioy P., et al. Personalized exposure assessment: promising approaches for human environmental health research. *Environ Health Perspect* 2005; 131: 840–848.
- Wilson N.K., Chuang J.C., Lyu C., Menton R., and Morgan M.K. Aggregate exposures of nine preschool children to persistent organic pollutants at day care and at home. *J Exp Anal Environ Epidemiol* 2003; 13: 187–202.
- Wu J., Fu Z.F., Yan F., and Ju H.X. Biomedical and clinical applications of immunoassays and immunosensors for tumor markers. *Trac-Trends Anal Chem* 2007a; 26: 679–688.
- Wu H., Liu G., Wang J., and Lin Y. Quantum-dots based electrochemical immunoassay of interleukin-1z. *Electrochem Commun* 2007b; 9: 1573–1577.
- Xiao Y., and Li C.M. Nanocomposites: from fabrications to electrochemical bioapplications. *Electroanalysis* 2008; 20(6): 646–662.
- Xu J.J., Wang A.J., and Chen H.Y. Electrochemical detection modes for microchip capillary electrophoresis. *Trac-Trends Anal Chem* 2007; 26: 125–132.
- Yantasee W., Lin Y., Hongsirikarn K., Fryxell G.E., Addleman R., and Timchalk C. Electrochemical sensors for the detection of lead and other toxic heavy metals: the next generation of personal exposure biomonitoring. *Environ Health Perspect* 2007a; 115(12): 1683–1690.
- Yantasee W., Timchalk C., and Lin Y. Microanalyzer for biomonitoring lead (Pb) in blood and urine. *Anal Bioanal Chem* 2007b; 387(1): 335–341.
- Zacco E., Galve R., Marco M.P., Alegret S., and Pividori M.I. Electrochemical biosensing of pesticide residues based on affinity biocomposite platforms. *Biosens Bioelectron* 2007; 22: 1707–1715.