



Cite this: *Analyst*, 2016, **141**, 1874

Received 15th December 2015,
Accepted 12th February 2016

DOI: 10.1039/c5an02572a

www.rsc.org/analyst

Paper-based analytical devices for environmental analysis

Nathan A. Meredith,^a Casey Quinn,^b David M. Cate,^{c,d} Thomas H. Reilly III,^{a,e} John Volckens^{*b,f} and Charles S. Henry^{*a,c,g}

The field of paper-based microfluidics has experienced rapid growth over the past decade. Microfluidic paper-based analytical devices (μ PADs), originally developed for point-of-care medical diagnostics in resource-limited settings, are now being applied in new areas, such as environmental analyses. Low-cost paper sensors show great promise for on-site environmental analysis; the theme of ongoing research complements existing instrumental techniques by providing high spatial and temporal resolution for environmental monitoring. This review highlights recent applications of μ PADs for environmental analysis along with technical advances that enable μ PADs to be more widely implemented in field testing.

^aDepartment of Chemistry, Colorado State University, Fort Collins, Colorado 80523, USA. E-mail: Chuck.Henry@ColoState.EDU

^bDepartment of Environmental and Radiological Health Sciences, Colorado State University, Fort Collins, Colorado 80523, USA. E-mail: John.Volckens@ColoState.EDU

^cDepartment of Biomedical Engineering, Colorado State University, Fort Collins, Colorado 80523, USA

^dIntellectual Ventures, Bellevue, Washington 98007, USA

^eAccess Sensor Technologies, LLC, Fort Collins, Colorado 80524, USA

^fDepartment of Mechanical Engineering, Colorado State University, Fort Collins, Colorado 80523, USA

^gDepartment of Chemical and Biological Engineering, Colorado State University, Fort Collins, Colorado 80523, USA

Recent outbreaks of food- and water-borne illnesses and sudden releases of toxic compounds into surface waters offer reminders of the importance of environmental monitoring for public health protection.^{1–3} Efforts to advance pollution monitoring have led to the development of many instrumented techniques capable of detecting parts per million (ppm) to parts per trillion (ppt) analyte concentrations in diverse sample matrices. To meet the needs of the monitoring community – namely, high sensitivity and low detection limits – most analytic methods rely on expensive equipment that require a high level of training to operate reliably. As a result, few methods have been developed that enable rapid, in-field detection. Furthermore, sampling and measurement costs



Nathan A. Meredith

Nathan Meredith received his B.S. in Chemistry and Mathematics from the University of Alabama in Huntsville in 2010. He went on to complete his Ph.D. in Chemistry (2015) at the University of Notre Dame where he studied neptunium incorporation into uranium(vi) compounds. He currently holds a postdoctoral position at Colorado State University and is investigating microfluidic paper-based analytical devices for the quantification of metals in environmental samples. In 2016, he will be joining the faculty at the University of Central Arkansas as an Assistant Professor in the Department of Chemistry.



Casey Quinn

Casey Quinn is an Industrial Hygiene PhD candidate in the Department of Environmental and Radiological Health Sciences at Colorado State University. He has Bachelors and Masters Degrees in Mechanical Engineering. His research is focused on the development and implementation of low-cost aerosol and water sampling devices which can be coupled with microfluidic paper-based analytical techniques for quantifying environmental contaminants.

associated with environmental monitoring often limit the sample size of the measurement, which in turn constrains our ability to define spatial and temporal patterns of contaminant release, transport, and fate. Ultimately, this lack of measurement resolution (due largely to cost, timeliness, and deployment limitations) hinders decision-making.

There is a growing need for low-cost technologies that can detect and monitor environmental contaminant concentrations quickly, easily, and in-field to provide timely data regarding the extent and magnitude of pollution. An enhanced understanding of the source, transport, and persistence of environmental contaminants could help prevent both human illness and ecosystem damage. Low-cost microfluidic paper-based analytical devices (μ PADs) offer an opportunity to address this need by increasing the frequency and geographic coverage of environmental monitoring while also reducing analytic costs and complexity of the measurement.


1. The rise of lab on paper

Various definitions of “microfluidic” exist throughout the literature; however, one common theme involves manipulating small volumes of fluids within micrometer-scale channels in engineered devices (e.g., not simple tubing).⁴ Microfluidic devices include those that are considered micro total chemical analysis systems (μ TAS), as well as more recent examples that range in capability from protein crystallization to point-of-care diagnostics.^{5–9} Chemically patterned paper was re-introduced in the last decade as an alternative to traditional microfluidic substrates (e.g. glass, silicon, and polymers) as a simple, low-cost platform. Paper and related porous hydrophilic materials offer many unique advantages over traditional microfluidic technologies such as power-free fluid transport *via* capillary action, high surface area to volume ratios for chemical reactions and detection, lightweight designs ($\sim 10 \text{ mg cm}^{-2}$), and the capacity for storing reagents in active form within the fiber network.^{10,11}

Paper has played a significant role in chemical analysis for many years; noted examples include litmus paper, home

pregnancy tests, sample filtration, and chromatography.^{12–16} As early as 23 to 79 A.D., paper saturated with extract from gall-nuts was used to detect ferrous sulfate in verdigris, the blue-green patina that follows the oxidation of copper, brass, and bronze surfaces.¹⁷ In the twentieth century, paper sensors were developed for chromatographic and electrophoretic separations as well as metals detection.^{18,19} In 2007, Martinez *et al.* reported the first μ PAD for multiplexed chemical analysis.²⁰ Such devices differ from traditional litmus paper or lateral-flow immunoassay methods in that chemical printing or cutting are used to define flow paths for conducting multiplexed analysis. For this review, we define a μ PAD as a device in which microliter volumes of sample are manipulated through a fibrous network by capillary action and where flow paths are defined by impermeable barriers or where the paper has been cut to create flow channels. Although the earliest μ PADs were developed for point-of-care clinical diagnostics, in recent years μ PADs have been used in other fields including environmental science. One of the first reported applications of μ PAD technology for an environmental sample was by Nie *et al.* in 2010 for electrochemical detection of Pb(II) and Zn(II).²¹ Since then, new μ PADs have been reported for a diverse range of contaminants in soil, water, air, and food.

Sensing devices made from paper have been featured in several reviews on microfluidics and advances in point-of-care diagnostics.^{4,22–27} The general science of μ PADs including theory, fabrication techniques, applications, and detection modes has been discussed in detail in a number of recent reviews dedicated specifically to μ PAD research.^{28–38} Other reviews have focused on applications for point-of-care medical diagnostics,^{39–44} electrochemical detection on paper,^{45,46} and on μ PADs as micro total analysis systems.^{28,47,48} To date, however, no review has focused exclusively on environmental applications, and this review seeks to address this important gap. First, we showcase multiple environmental applications of μ PADs, categorized by analyte class. Next, the discussion is broadened to include recent trends in μ PAD technology toward field deployment and how these developments might impact environmental monitoring. Finally, we revisit some of the

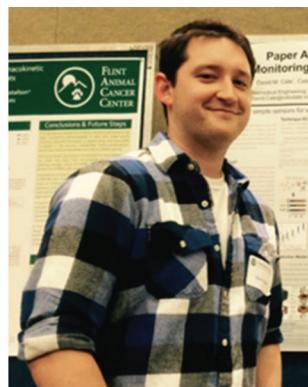

David M. Cate

David Cate is a biomedical engineer at Intellectual Ventures Lab/Global Good, USA. He received his Ph.D. in bioengineering from Colorado State University in 2015, where he worked on developing inexpensive paper sensors for measuring metal particulates in occupational environments. His current work is focused on creating lateral flow immunoassays for point-of-care malaria elimination campaigns.



Thomas H. Reilly III

Dr Reilly earned his B.S. degree from Boston College and Ph.D. from the University of Colorado. He has worked on projects related to molecular spectroscopy, materials science, solar energy conversion, sensors and instrument development. He is currently employed at Access Sensor Technologies where he is commercializing μ PADs for environmental analysis applications.

challenges of employing μ PADs for environmental monitoring and include a perspective on future directions in the field.

2. Applications

Analytes for environmental μ PADs can be roughly grouped into three classes – inorganic (metals, non-metals such as phosphate), organic (small molecules, pesticides, *etc.*), and biological (bacteria, *etc.*) – or by specific applications (explosives, oxidative reactivity, *etc.*), based on the literature published to date. For each analyte class or application presented below, a general overview is provided followed by an in-depth discussion of seminal works.

Analyte quantification with μ PADs is commonly achieved using colorimetric (intensity/hue-, count-, distance-, or time-based), electrochemical, fluorescent, or electrochemiluminescent methods. Although colorimetric analysis is most common because of its simplicity, the method can suffer from low signal sensitivity and can be inadequate for point-of-need environmental analysis without additional sample preparation steps (*e.g.* analyte preconcentration, matrix simplification, *etc.*). Low-cost fabrication methods for more sensitive electrochemical techniques (employing carbon paste or metal micro-wire electrodes) have opened the door for this technology to become a viable alternative to colorimetric detection on paper sensors.⁴⁶ The sensitivity and specificity of electrochemistry on paper can compete with traditional benchtop techniques like UV-Vis spectroscopy, liquid chromatography, and inductively coupled plasma-mass spectrometry. Developing multiplexed tests may be key for electrochemical systems to find success in future commercial markets. One drawback of electrochemical sensing is the need for potentiostats, however small they may be, which can lead to increased costs for analysis relative to colorimetric systems read by the naked eye.



John Volckens

John Volckens is an associate professor of Mechanical Engineering and the Director of the Center for Energy Development and Health at Colorado State University. He also holds appointments in the Department of Environmental and Radiological Health Sciences, the School of Public Health, and the School of Biomedical Engineering. His research interests involve combustion and aerosol science, sensor technology, and air pollution-related disease. He earned a B.S. in Civil/Environmental Engineering from the University of Vermont and his M.S. and Ph.D. degrees from the University of North Carolina at Chapel Hill.

lution-related disease. He earned a B.S. in Civil/Environmental Engineering from the University of Vermont and his M.S. and Ph.D. degrees from the University of North Carolina at Chapel Hill.

2.1 Metals

Human exposure to metals has been established as a contributor to morbidity and mortality, especially in regions lacking strict regulations for metal contamination of water, soil, and/or air.^{49,50} Redox active metals like Fe, Cu, Cr, and Co possess the ability to generate free radicals that can cause oxidative stress in organisms,⁵¹ while metals like Pb and Cd are well known neurotoxins.^{52,53} Human exposure to metals is associated with many diseases, but ongoing efforts to identify exposure sources are hindered by the cost of measurement; routine analysis often exceeds \$100 per sample, resulting in limited measurement campaigns. The spatial and temporal distribution of measurement can also be important for understanding the source (or spread) of a pollutant and for tracking its impact on people, wildlife, and the environment. After three million gallons of polluted mine waste containing Co, As, Ni, and Cr from the Gold King Mine was accidentally released into the Animas River in Colorado (2015), reliable information regarding pollution levels was scarce for many days. At the time of the spill, little was known about the concentrations of the metals in the river, which generated a significant public outcry.²

Since 2010, metal quantification with paper-based sensors has attracted attention because colored metal-ligand complexes are easily discernable with the unaided eye and/or can be quantified inexpensively with other optical motifs (*e.g.* scanner or camera-phone). Additionally, much of the complexation chemistry is well-characterized.⁵⁴ One of the first examples of μ PAD-based quantification of metals was a sensor comprised of four detection zones for simultaneously measuring Fe, Cu, and Ni from medical incineration ash.⁵⁵ Detection limits for this type of particulate matter ranged from 1–1.5 μ g (total mass on device) for each analyte. Colorimetric detection of total Cr and Cr(vi) from ash and welding fume samples has also been reported in devices with similar architecture.^{56,57}



Charles S. Henry

Charles S. Henry received his B.S. degree in Chemistry from Missouri Southern State College Ph.D. in Analytical Chemistry from the University of Arkansas followed by postdoctoral studies as an NIH postdoctoral fellow at the University of Kansas. He started his academic career at Mississippi State University before moving to Colorado State University in 2002. He is currently full professor and department chair of Chemistry at Colorado State University and also serves as a faculty member in Chemical & Biological Engineering and Biomedical Engineering. His research group focuses on developing new sensors and separation systems using lab-on-a-chip methods.

Paper devices for measuring Zn, Cu, Ag, Cd, Pb, Ni, Hg, and Cr(vi) colorimetrically have been developed with detection limits in the tens to hundreds of ppm using metal-to-ligand charge-transfer chemistry.^{58–70} A fluorogenic method for measuring Hg and Cr(III) has also been reported.⁷¹ In the absence of sample preconcentration, however, many colorimetric methods are limited to ppm-level detection limits, which can be inadequate for some point-of-need scenarios requiring ppb-level detection limits. Electrochemical detection, on the other hand, has demonstrated the capability to quantify metals in water at sub-ppb levels.^{21,72}

Hybrid μ PADs that combine detection motifs, such as colorimetry and electrochemistry, are potentially advantageous because environmental contaminants are often present at concentrations that differ by several orders of magnitude through space and time; a single technique may not be suitable for measuring all analytes in the same matrix.⁷² In a recent publication, Rattanarat *et al.*⁷³ created a three-dimensional μ PAD (Fig. 1A) that combined colorimetric and electrochemical detection on separate layers for quantifying Ni, Cu, Fe, Pb, Cr(vi), and Cd using a small punch (10 mm diameter) taken from an air sampling filter. The technique was developed for contaminants present in airborne particulate matter. Sample flowed laterally on the top layer of the device in four segregated channels enabling colorimetric determination of Cu, Ni, Fe, and total Cr. These metals were measured colorimetrically because they are often present at higher (ppm) concentrations in the environment. Sample also flowed vertically to a second layer where Pb and Cd were quantified electrochemically. Separating the detection modes *via* multiple layers was necessary to minimize cross-contamination; distinct reaction chemistry (e.g. agent masking, pH adjustments) also enhanced analyte selectivity and sensitivity. For example, interference from Cu during anodic stripping voltammetry of Cd and Pb was minimized by adding a Cu-complexing agent, ferricyanide, to the electrochemical layer without impeding the colorimetric detection of Cu in the top layer. Detection limits as low as 0.75 μ g (15 ppm) for Fe, Ni, and Cu, 0.12 μ g (2.4 ppm) for Cr(vi) and 0.25 ng (50 ppb) for Cd and Pb were reported.

2.2 Non-metals

Health concerns associated with exposure to many non-metal inorganic compounds have led to environmental regulations and policies for establishing permissible exposure concentrations. For example, excess nitrogen and phosphorus in surface and groundwater are precursors to algal blooms (cyanobacterial toxins)^{74,75} and conditions such as methaemoglobinemia (blue baby syndrome).^{76,77} These inorganic contaminants are released into the environment as combustion byproducts, in agricultural runoff, and in other sample matrices from animal production facilities. Chloride and fluoride, which are intentionally added to drinking water for health reasons, can negatively impact human health if ingested concentrations are too high.^{78,79} Cyanide, which is extremely toxic, is released into the environment from natural deposits,

mining operations, orchards, biomass combustion, and waste streams from glass and electronics production.^{80,81}

A number of low-cost assays, including μ PADs, have been developed for measuring inorganic compounds in the environment. Numerous μ PAD papers have described the colorimetric determination of phosphate,⁸² nitrate,^{83–89} nitrite,^{83–91} ammonia,^{92,93} arsenic,⁹⁴ and cyanide.⁹⁵ A paper device capable of performing an acid–base titration has been applied to the measurement of water pH in an acidic hot spring.⁹⁶ Electrochemical detection of iodide,⁹⁷ bromide,⁹⁷ chloride,^{97–100} potassium,¹⁰⁰ and ammonium¹⁰⁰ has been demonstrated on a μ PAD using potentiometry, where the potential difference between a reference and indicator electrode was indicative of analyte concentration. The majority of these publications only focus on the development of novel μ PAD designs and benchtop fabrication techniques; few publications have reported on method validation in the field (or with real-world samples analyzed in the lab).

Jayawardane *et al.* published a series of papers describing novel approaches for detecting reactive ammonia/ammonium cation,⁹³ phosphate,⁸² and nitrite/nitrate⁸⁹ in water using three-dimensional μ PADs. Sodium hydroxide was used to convert ammonium cations to ammonia, and a hydrophobic microporous Teflon membrane separated ammonia from the remaining ammonium cations by gaseous diffusion (Fig. 1B). The ammonia content was quantified using the acid–base indicators 3-nitrophenol and bromothymol blue giving detection limits of 0.8 and 1.8 mg N L⁻¹, respectively. The phosphate μ PAD (Fig. 1C) used the phosphoantimonyl-molybdenum blue complex and had a working detection range of 0.2–10 mg L⁻¹. Notable to this design was the inclusion of a PTFE or cellulose acetate sheet that was removed immediately prior to use for improving device shelf-life. The nitrate/nitrite μ PAD (Fig. 1D) was able to detect nitrite concentrations down to 1.0 μ M using the Griess reaction. Total nitrate/nitrite levels were also quantifiable using zinc particles to reduce nitrate to nitrite. To their knowledge, this was the first application of solid-phase reagents in a modern μ PAD. Each of these devices and their detection methodologies were tested with lab standards and environmental water and wastewater samples. The μ PAD assays were also validated against traditional spectroscopic methods, ion chromatography, or flow injection analysis.

2.3 Organic molecules

Exposure to environmentally persistent organic pollutants has numerous adverse health effects depending on the mechanism of action (e.g., xenoestrogenic, carcinogenic, mutagenic, *etc.*) or the impacted organs.^{101–103} Paper-based sensors have been reported for the detection of chemical warfare agents,¹⁰⁴ recreational drugs,¹⁰⁵ volatile organic compounds (VOCs),^{106–109} and phenolic compounds.^{110–113} Detection of chemical warfare agents and recreational drugs is more appropriately described as a forensic rather than an environmental application and will not be discussed here. Several μ PAD procedures for the detection of VOCs have been published using both colori-

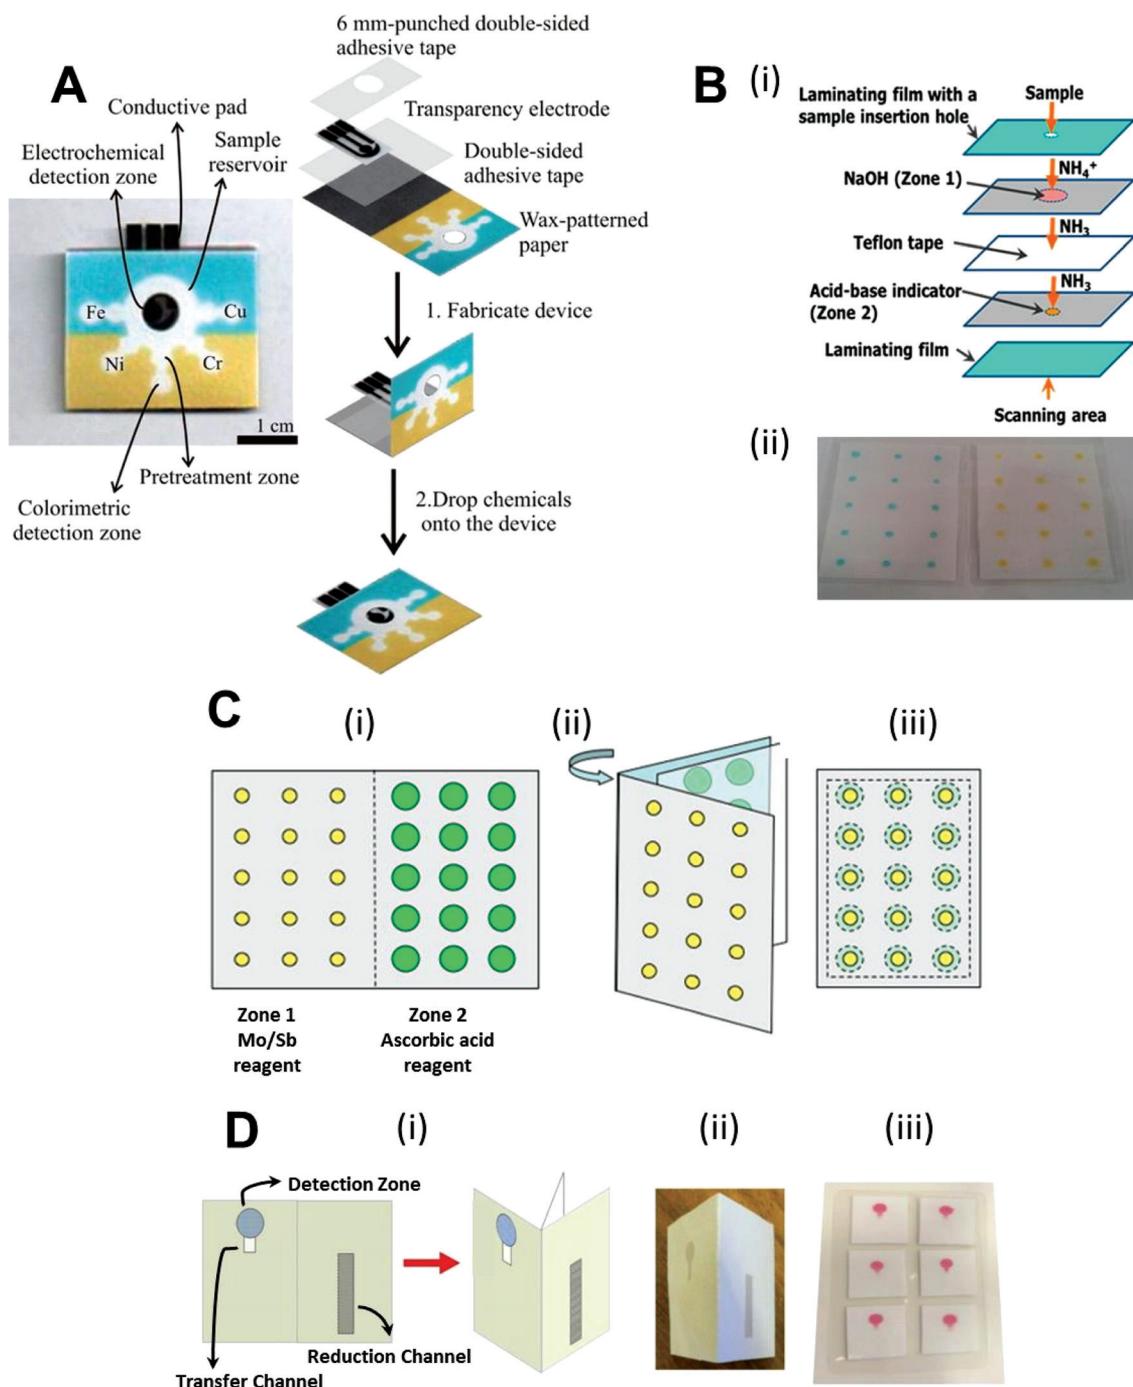


Fig. 1 Examples of μPADs for inorganic species. (A) Three-dimensional hybrid colorimetric/electrochemical μPAD for simultaneously determining Fe, Ni, Cu, Cr, Cd, and Pb. Reproduced with permission from ref. 73. Copyright 2014 American Chemical Society. (B) Multilayer device for quantifying ammonia using pH indicators. Adapted with permission from ref. 93. Copyright 2015 American Chemical Society. (C) μPAD for measuring reactive phosphate; a removable sheet was placed between paper layers to improve shelf life. Adapted from ref. 82 with permission from Elsevier. (D) μPAD for measuring nitrate and nitrite. Adapted with permission from ref. 89. Copyright 2014 American Chemical Society.

metric^{106,108,109} and electrochemical detection.¹⁰⁷ Notably, Soga *et al.* developed a colorimetric sensor capable of selectively discriminating volatile primary amines from other common VOCs.¹⁰⁸

Although VOCs are environmentally important contaminants, μPADs for detecting these compounds are in the early

stages of development. Phenolic compounds, on the other hand, have been more widely measured using both electrochemical^{111–113} and colorimetric¹¹³ detection techniques. Due to their potential bioaccumulation in the environment and their wide-ranging human and ecological health impacts, phenolic compounds pose a significant risk.^{114–117}

The first reported μ PAD for the detection of environmental phenolic compounds was published by Alkasir *et al.* (Fig. 2A).¹¹⁰ Their device was constructed using layer-by-layer deposition of chitosan, tyrosinase, and sodium alginate onto filter paper. The alginate and chitosan layers electrostatically trapped tyrosinase. The immobilized enzyme oxidized the aromatic phenol to a corresponding ketone which, in turn, selectively bound to the amino functionality of the chitosan layer producing a color change. The device was applied to the detection of phenol, bisphenol-A (BPA), *m*-cresol, *p*-cresol, catechol, and dopamine. Most reagents were identified by the formation of a red-brown product; however, addition of BPA resulted in a blue-green color. The number of layers, pH, and reagent amounts were optimized resulting in a detection limit of $0.86 \pm 1 \mu\text{g L}^{-1}$ for the phenolic compounds tested. Cross-reactivity was not observed for ascorbic acid, uric acid, and phenylalanine. Devices were tested with BPA spiked tap and river water samples to evaluate their effectiveness in real matrices. Furthermore, the device showed room temperature stability

over 260 days. A scaled-up manufacturing method was presented in which the layer-by-layer deposition was achieved using inkjet printing. In a subsequent work,¹¹⁸ the authors presented a portable device using the same sensor to conduct field measurements of BPA in indoor dust. The device consisted of an air-sampler interfaced with a test zone containing interchangeable paper sensors. The procedure was validated alongside traditional gas chromatography methods. The detection limit for the sensor was $0.28 \mu\text{g g}^{-1}$ which is similar to the established United States Environmental Protection Agency reference dose of $50 \mu\text{g per kg BW per day}$.¹¹⁸

2.4 Pesticides

Pesticides are well-known toxins found in air, water, soil, food, and feed products.¹¹⁹ Exposure can occur *via* ingestion, inhalation, and dermal absorption and is associated with neurotoxicity, hepatotoxicity, renal toxicity, dermatitis, and cancer.^{120–122} Separation methods like gas and high-pressure liquid chromatography are commonly applied techniques for

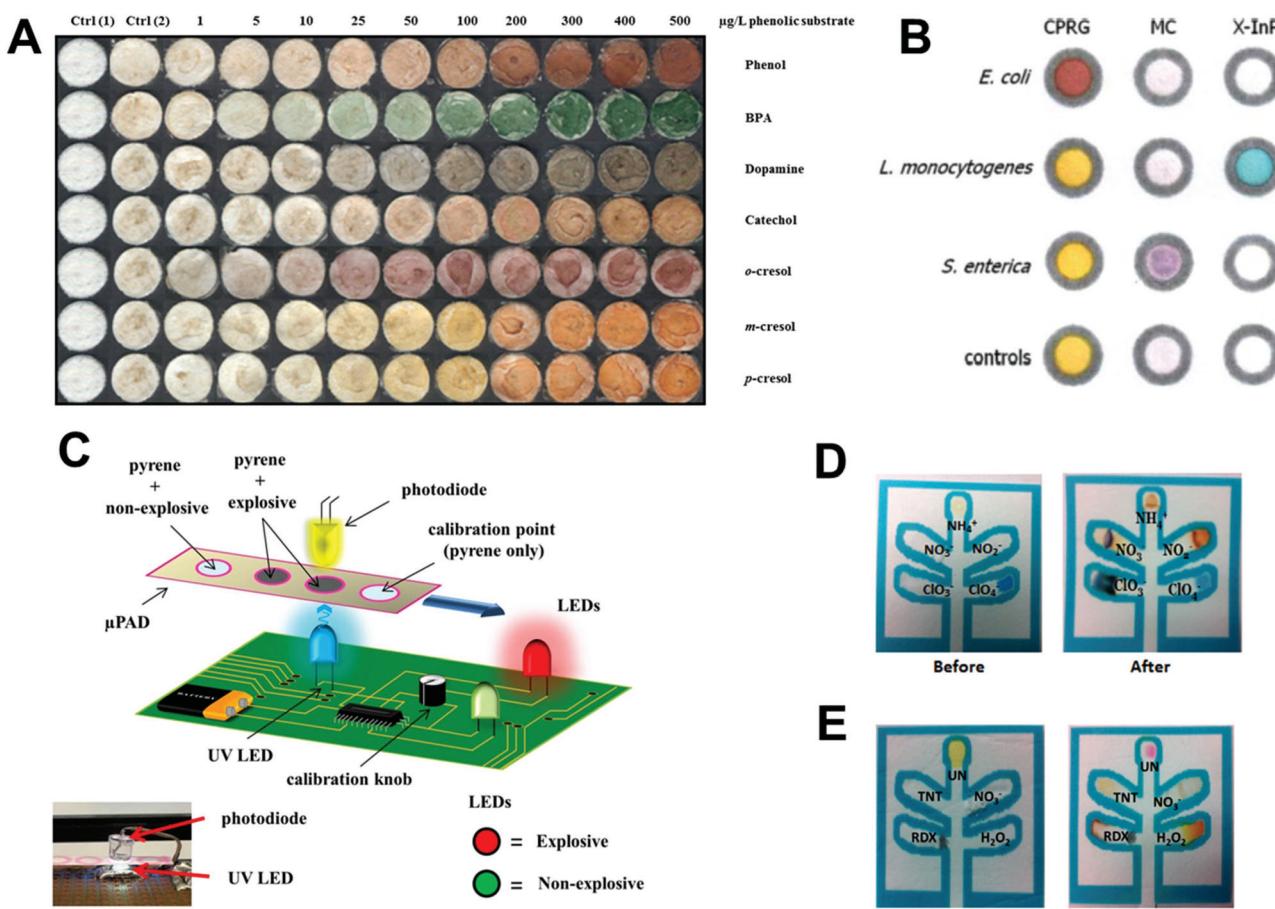


Fig. 2 Examples of μ PADs for organic species, bacteria, and explosive compounds. (A) Tyrosinase-based μ PAD for detecting phenolic compounds. Reprinted with permission from ref. 110. Copyright 2012 American Chemical Society. (B) Spot tests for three bacterial strains showing lack of interference. Reprinted with permission from ref. 141. Copyright 2012 American Chemical Society. (C) Schematic of a handheld fluorescence detector used to measure fluorescence quenching of pyrene by explosive compounds. Reproduced from ref. 147 with permission from The Royal Society of Chemistry. (D) Colorimetric μ PAD for detecting inorganic explosives. Adapted from ref. 150 with permission from The Royal Society of Chemistry. (E) Colorimetric μ PAD for organic and high explosives. Adapted from ref. 150 with permission from The Royal Society of Chemistry.

sensitive and selective determination of pesticides, but analysis is expensive and not well suited for on-site measurement, particularly in remote regions or for situations requiring rapid screening. Alternatively, μ PADs offer a practical, cost-effective means of rapidly analyzing food products for pesticides.

Many μ PAD-based efforts for identifying or detecting pesticides are based on the inhibition of acetylcholinesterase (AChE), an enzyme critical for controlling normal transmission of nerve impulses.^{123–125} Normally, acetylcholine is broken down by AChE into choline and acetic acid, but the presence of organophosphate, organophosphorus, and carbamate pesticides is inhibitory.^{126–128} Measuring AChE inhibition levels by pesticides has been accomplished using chemiluminescence,^{129,130} electrochemistry,¹³¹ and colorimetry with immobilized organic molecules^{132–134} and semiconductor quantum dots.^{123,135} Dichlorvos (2,2-dichlorovinyl dimethylphosphate), a highly toxic organophosphate pesticide widely used for crop protection,¹³⁶ has been measured with μ PADs at levels as low as 0.8 ppb.^{129,137} In 2009, Hossain *et al.*¹³⁸ developed a multiplexed sensor for rapidly (~5 min) measuring acutely toxic organophosphate insecticides like bendiocarb (0.2 ppb), carbaryl (2 ppb), paraoxon (0.3 ppb), and malathion (3 ppb) based on AChE inhibition. The colorimetric reagent, indophenyl, produced a yellow to blue color shift in basic solution upon AChE-catalyzed hydrolysis of indophenyl, forming the indophenoxy anion. Color intensity was inversely proportional to analyte concentration. Lateral-flow and dipstick formats were developed where the analyte was measured with and without incubation. In the lateral-flow format, a pipette was used to deliver the analyte to the device. For the dipstick device, one end of the sensor was immersed in a container filled with the sample. Pesticide residues collected from apples and lettuce were in agreement with conventional analytical methods and matrix effects from spiked milk and juice were negligible.

2.5 Bacteria

The use of μ PADs for the detection of bacterial contamination in environmental samples, notably food and water, is driven by the need for faster, simpler, lower cost methods in both developing and developed nations.^{139–143} Traditional measurements involve sending samples to a centralized laboratory for culture analysis or molecular detection (polymerase chain reaction, enzyme-linked immunosorbent assay), neither of which is suitable for routine monitoring due to the cost, analysis times, and need for highly trained personnel. A μ PAD platform, on the other hand, offers low-cost, on-site, analysis with relatively rapid turnaround relative to traditional methods. Three main strains of bacteria have been investigated in environmental samples with μ PADs: *Escherichia coli*,^{139–141,143} *Listeria monocytogenes*,^{141,142,144} and *Salmonella*.^{141,145} Frequently reported detection motifs use colored enzymatic assays on modified bioactive paper,^{139–143} light scattering,¹⁴⁵ and chemiluminescence.^{139,144}

In 2012, Jokerst *et al.* developed a series of paper-based spot tests for the colorimetric enzymatic determination of

E. coli, *L. monocytogenes*, and *S. enterica* in ready-to-eat meat (Fig. 2B).¹⁴¹ In this report, enzymes produced by bacteria during growth in culture media reacted with compounds pre-deposited (and dried) on the μ PAD. *E. coli* determination was based on the yellow to red color change produced between β -galactosidase and chlorophenol red β -galactopyranoside. *L. monocytogenes* detection was achieved by the reaction between phosphatidylinositol-specific phospholipase C and 5-bromo-4-chloro-3-indolyl-*myo*-inositol phosphate, which was characterized by the appearance of a blue color. Finally, *S. enterica* was determined using the reaction between esterase and 5-bromo-6-chloro-3-indolyl caprylate to produce a purple color. Limits of detection were on the order of 10 colony forming units per cm^2 (cfu cm^{-2}) from a surface swab after 4–12 hours of enrichment which is significantly faster than standard culture techniques. The devices were optimized based on enzyme and substrate concentrations, total well volume, sonication time, and cross-reactivity. Finally, the authors inoculated ready-to-eat meats¹⁴¹ and samples of irrigation water¹⁴⁶ to demonstrate method applicability for food safety and environmental monitoring.

In another notable paper from the same year, Hossain *et al.* demonstrated a multiplexed device for the specific detection of non-pathogenic and pathogenic *E. coli*.¹⁴⁰ Non-pathogenic *E. coli* was detected from the reaction of 5-bromo-4-chloro-3-indolyl- β -D-glucuronide sodium salt in the presence of β -glucuronidase, which produced the highly colored indolyl species and glucuronide. Total *E. coli* was indicated using the same β -galactosidase chemistry described above. Moreover, the authors demonstrated the use of immunomagnetic nanoparticles to concentrate *E. coli* by means of a magnetic separation step without the need for external cell culturing. The influence of other components in the sample matrix was tested with artificially contaminated samples of orange juice and milk. The specificity of the device was confirmed against the presence of *Bacillus subtilis* and *S. enterica* in the liquid test samples. The detection limits for pathogenic and non-pathogenic *E. coli* were 5 and 20 cfu mL^{-1} , respectively.

2.6 Explosives

Pre- and post-detonation screening of explosives is interesting to environmental science because compounds in explosives have relatively slow decomposition in soil, which can lead to water contamination.¹⁴⁷ Several articles have been published on explosives analysis with μ PADs using fluorescence,^{147,148} colorimetry,^{149–152} and surface-enhanced Raman spectroscopy.¹⁵³ Most μ PADs for detecting explosives have focused on nitroaromatics;^{148,149,153} however, recent efforts have focused on the development of μ PADs capable of simultaneous, multiplexed detection of a wide range of compounds including both inorganic and organic explosives.^{147,150,151}

In 2013, Taudte *et al.* developed a μ PAD for measuring compounds in explosives *via* fluorescence quenching of pyrene.¹⁴⁷ The poor water solubility of pyrene coupled with the incompatibility of organic solvents and wax barriers were addressed by testing different waxes (e.g. colors) and barrier

thicknesses along with mixed solvent systems. A 80:20 methanol:water mixture was suitable for dissolving pyrene and showed minimal penetration of the wax barriers. Device performance was evaluated with 10 different compounds including nitrate esters, nitroaromatics, and nitro amines, all of which led to fluorescence quenching of pyrene. While not specific to a particular compound, the method was selective for explosive *versus* non-explosive samples such as water, milk, or coffee, based on differences in fluorescence quenching. The authors also developed a small, portable fluorescence detector for in-field use (Fig. 2C). The prototype reader had comparable performance to the benchtop instrument used for method validation.

Peters *et al.* detailed simultaneous colorimetric detection of a series of inorganic and organic compounds found in improvised explosive devices.¹⁵⁰ Previously reported μ PADs focused on a subset of explosives; however, this was the first device capable of multiplexed detection of different explosive compounds. Two distinct μ PADs were prepared (Fig. 2D and E) – the first for detection of inorganic explosives (chlorate, nitrate, ammonium, nitrite, and perchlorate) and the second for detecting a mixture organic and inorganic explosive compounds (nitroamines, trinitroaromatics, urea nitrate, nitrate, and hydrogen peroxide). Several interferences were tested and no false positives or false negatives were observed. Additionally, black powder and fireworks were also tested to demonstrate the device performance on real samples.

2.7 Oxidative activity

Oxidative stress in living organisms, a phenomenon that has been linked to aging and disease, can occur following exposure to reactive oxygen species (ROS).^{154–157} Common ROS are redox active metals, superoxides, hydroxide radicals, small organic molecules (*e.g.* quinone family), and enzymes. Some ROS are generated within living cells as products of natural metabolism, but more recent interest has focused on exposure to ROS from environmental sources as these compounds may overwhelm the body's natural ability to manage oxidative stress. Given the wide range of species that fall under the category of ROS it is necessary to find an assay that can serve as an approximate gauge of the total ROS activity found in environmental samples.

Mani *et al.* developed a field-deployable μ PAD to detect oxidative DNA damage using Cytochrome P450 enzymes to metabolize environmental toxins into reactive metabolites.¹⁵⁸ The metabolites reacted with co-immobilized DNA causing it to partially unfold. The degree of unfolding was proportional to the toxin level. An electrochemiluminescent signal was generated when (bis-2,2'-bipyridyl) ruthenium polyvinylpyridine $[[\text{Ru}(\text{bpy})_2(\text{PVP})_{10}]]^{2+}$ polymer reacted with exposed guanines. The signal increased based on the extent of DNA damage, due to the increased availability of guanines in DNA to react with the Ru(III). As is common with ROS studies, a suitable external standard was needed to compare the oxidative activity among heterogeneous samples. Mani *et al.* found that benzo-[*a*]-pyrene was a suitable model oxidant and converted

genotoxicity of their samples to a benzo-[*a*]-pyrene equivalent. The technique was demonstrated by analyzing smoke, water, and cooked food samples.

Dithiothreitol (DTT) oxidation is also used to gauge the oxidative reactivity of analytes in environmental samples.^{155,159–162} In this assay, DTT is oxidized by ROS in samples (*e.g.* fluid extracts from air filter media) for a fixed period of time. After reacting with the sample, remaining (unconsumed) DTT is reacted with 5,5'-dithiobis-2-nitrobenzoic acid (Ellman's Reagent) to yield the yellow 2-nitro-5-thiobenzoate dianion. The color intensity of this dianion is inversely related to the ROS activity of the sample. The DTT assay has been demonstrated on μ PADs for air samples collected in close proximity to a wildfire, on a clear day, and from a commercial kitchen.¹⁶² Other colorimetric assays based on tris(2-carboxyethyl)phosphine (TCEP) or the aggregation of silver nanoparticles in the presence of reduced glutathione have been reported.^{163,164}

3. Current limitations and recent trends

Despite the promises of low-cost, small sample and reagent volumes, portability, and rapid response time, μ PADs, in their current state, must overcome several limitations that inhibit their widespread application in the field. Large-scale field demonstrations of μ PAD capabilities have been limited; one of the few examples to date was a biomedical test for the detection of transaminase as an indicator of drug-induced liver injury.¹⁶⁵ Although some studies using environmental μ PADs have reported the analysis of real-world samples brought back to the lab, these were, for the most part, small-scale studies, and the devices have not yet reached the same state of field readiness as their biomedical counterparts. One notable exception is the recent work of Sicard *et al.*¹³³ Their preliminary experiments coupled the detection of organophosphate pesticides on a paper sensor with analysis using a smartphone. After each analysis, the result, date, and location were uploaded to a central web server using the smartphone's GPS system. The advantages afforded by this technique for collaborative mapping may be applied to long-term or large-scale environmental monitoring of contamination hotspots or as a means for early detection.

On-site analysis is important for widespread deployment of a rapid response test. Perhaps the most straightforward (and inexpensive) method for target determination has been colorimetric detection. If performed entirely visually (*i.e.* without any optical instrumentation), differentiation of color intensity is semi-quantitative and has been shown to vary from person-to-person^{64,166} Colorimetric detection aided by a scanner or camera for image acquisition can improve method accuracy (Fig. 3A), but increases analysis costs and could limit field use. Recently, groups have reported semi-quantitative alternatives to intensity-based colorimetry such as count-, distance-, and time-based μ PADs that eliminate the need for imaging. In

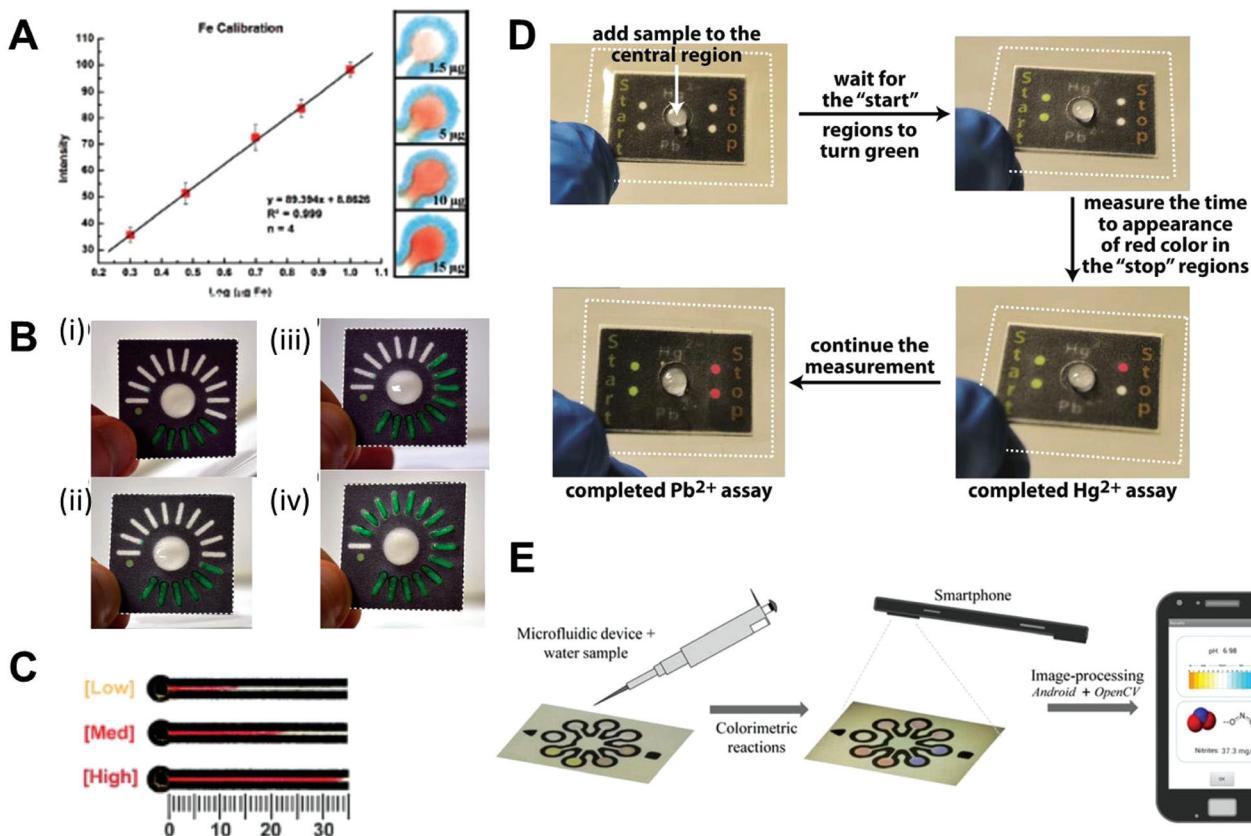


Fig. 3 Quantitative methods commonly used with colorimetric assays on μ PADs. (A) Calibration curve for intensity-based analysis of a scanned device using ImageJ. Reprinted with permission from ref. 55. Copyright 2012 American Chemical Society. (B) Count-based quantitation achieved by counting the number of colored tabs. Adapted from ref. 167 with permission from John Wiley and Sons. (C) Distance-based detection by measuring the length of color development along a channel. Reproduced from ref. 68 with permission from The Royal Society of Chemistry. (D) Time-based quantification. Reproduced from ref. 169 with permission from The Royal Society of Chemistry. (E) Use of a smartphone to conduct intensity-based measurements. Reprinted with permission from ref. 88. Copyright 2014 American Chemical Society.

count-based detection, concentration is determined by counting the number of bars, tabs, or spots that develop color (Fig. 3B).¹⁶⁷ Distance-based quantification is achieved by measuring the distance of continuous color development along a channel with an on- or off-device ruler (Fig. 3C).^{68,69} Time-based quantification correlates concentration to the time difference for color development between a test zone and control zone (Fig. 3D).^{168,169}

Similarly, many μ PAD-based electrochemical assays rely on expensive (>\$10 000) desktop potentiostats for analysis. If the capabilities of μ PADs are to be reached, the cost of electrochemical detectors will need to be reduced. Fortunately, in the last few years, several groups have reported new handheld units capable of measuring single ppb levels of analyte for a fraction of the price of traditional units.^{170–173} One example is the CheapStat, which is an inexpensive (<\$80), open-source hardware and software potentiostat.¹⁷⁰ On-going work will continue to drive down the cost of handheld sensors which will rapidly expand the utility and reach of μ PAD-based electrochemical systems.

Worldwide distribution of smartphones and camera phones has significantly decreased the cost of sensor develop-

ment because the phone becomes the detector and source of data transmission. For example, new software programs have been developed for conducting intensity-based colorimetric measurements in the field using a smartphone.^{88,133,166,170,174–182} Lopez-Ruiz *et al.* recently described a colorimetric μ PAD for simultaneously evaluating pH and nitrite concentration in water (Fig. 3E).⁸⁸ A custom smartphone application was used to photograph the μ PAD, and a software algorithm correlated hue–saturation–brightness indices with solution pH and nitrite concentration. Park *et al.* expanded this method by developing an application to indicate the optimal angle and distance from the user to the completed device.¹⁴⁵ Smartphone analysis has also been applied to electrochemical measurements on μ PADs. For example, Delaney *et al.* recently reported a procedure in which they used a smartphone as a potentiostat by controlling the amplitude and waveform of the audio output.¹⁷⁵ Additionally, quick response (QR) codes have been implemented in some devices and could be used in the future to share vital diagnostic/identifier information about the sample without requiring user input. This sample identification would help automate and improve field data collection.^{111,183} Future examples utilizing

smartphone technology will continue to revolutionize μ PAD applications, enabling further field deployment.

4. Conclusions

Although μ PADs were originally developed as biomedical assays for point-of-care diagnostics,²⁰ their use has expanded into environmental research. By comparison to the progress achieved in biomedical devices, environmental monitoring with μ PADs is still a nascent field of research. Guidance for the development of new applications may be taken from environmental and public health concerns highlighted by the World Health Organization (WHO),¹⁸⁴ the Environmental Protection Agency (EPA),^{185–187} and other similar organizations from around the world.

The research highlighted in this review demonstrates that μ PADs can successfully detect environmental contaminants; however, there is still a need for further developments to improve sensitivity and for field validation. The field-readiness of existing μ PAD assays can be assessed in terms of established regulatory limitations and standards. For example, the Occupational Safety and Health Administration (OSHA) limits personal exposure to Cu in air at 1.0 mg m^{-3} .¹⁸⁸ The corresponding EPA regulation for Cu in drinking water is 1.3 mg L^{-1} (1.3 ppm).¹⁸⁹ Rattanarat *et al.*⁷³ reported a LOD of 15 ppm for Cu by colorimetric methods indicating a need for improvement since method sensitivity falls above regulatory limits for drinking water. By contrast, the LOD for nitrite by Jayawardane *et al.*⁸⁹ of $1.0 \mu\text{M}$ (0.046 ppm) is well within the EPA limit of 1 mg L^{-1} (1 ppm).¹⁸⁹ Due to the diversity of μ PAD techniques and variability in regulatory limits for a given analyte, which depend on the sample matrix and the regulating agency, the field-readiness of environmental μ PADs needs to be considered on a case-by-case basis, which is beyond the scope of the present review.

In addition to meeting regulatory limits, the successful commercialization of μ PAD technologies may require the design of devices capable of measuring multiple analytes.^{10,69,70,73,140} One particular challenge presented by environmental monitoring is that analyte concentrations can vary by orders of magnitude in space and time. Devices, such as the dual colorimetric-electrochemical μ PAD designed by Rattanarat *et al.* for quantifying metals show promise for meeting this challenge.⁷³ Multimodal detection strategies are useful because colorimetric analysis, can achieve ppm sensitivity whereas electrochemistry can detect analytes with ppb sensitivity. In certain situations, it may be more advantageous to utilize one detection motif over others. By integrating portable electrochemical analyzers, hybrid-detection mode μ PADs have the potential to become very powerful tools for in-field, long-term environmental monitoring.

Environmental μ PADs are not likely to replace existing instrumented environmental monitoring techniques, rather they will likely serve as a facile means of complementing current methodology. The low cost and rapid detection time of

μ PADs have the potential for widespread routine monitoring over large geographic areas and for long time periods providing thousands of individual measurements. Moreover, the recent developments towards improving the distribution and usability of environmental μ PADs may provide the growing field of citizen science with a new set of tools and more readily involve citizens in the protection and improvement of human and environmental health. These measurements may ultimately provide better profiling of spatial and temporal variations in pollutant levels on a scale that has not been previously possible.

References

- 1 Centers for Disease Control and Prevention, *Listeria* outbreaks, <http://www.cdc.gov/listeria/outbreaks/>, (accessed December, 2015).
- 2 United States Environmental Protection Agency, Emergency response to August 2015 release from gold king mine, <http://www.epa.gov/goldkingmine>, (accessed December, 2015).
- 3 United States Environmental Protection Agency, Deep-water horizon – BP Gulf of Mexico oil spill, <http://www.epa.gov/enforcement/deepwater-horizon-bp-gulf-mexico-oil-spill>, (accessed December, 2015).
- 4 A. Gencoglu and A. R. Minerick, *Microfluid. Nanofluid.*, 2014, **17**, 781–807.
- 5 A. Manz, N. Gruber and H. Widmer, *Sens. Actuators, B*, 1990, **1**, 244–248.
- 6 S. Haeberle and R. Zengerle, *Lab Chip*, 2007, **7**, 1094–1110.
- 7 G. M. Whitesides, *Nature*, 2006, **442**, 368–373.
- 8 D. Mark, S. Haeberle, G. Roth, F. von Stetten and R. Zengerle, *Chem. Soc. Rev.*, 2010, **39**, 1153–1182.
- 9 C. D. Chin, V. Linder and S. K. Sia, *Lab Chip*, 2007, **7**, 41–57.
- 10 K. Abe, K. Suzuki and D. Citterio, *Anal. Chem.*, 2008, **80**, 6928–6934.
- 11 J. L. Delaney, C. F. Hogan, J. Tian and W. Shen, *Anal. Chem.*, 2011, **83**, 1300–1306.
- 12 J. Davy, Abstracts of the papers printed in the Philosophical Transactions of the Royal Society of London, 1800.
- 13 K. Dieterich, *US Pat.*, US 691249A, 1902.
- 14 H. Yagoda, *Ind. Eng. Chem., Anal. Ed.*, 1937, **9**, 79–82.
- 15 P. W. West, *Ind. Eng. Chem., Anal. Ed.*, 1945, **17**, 740–741.
- 16 H. Weil, *Kolloidn. Z.*, 1953, **132**, 149–162.
- 17 J. Partington, *J. Roman Stud.*, 1929, **19**, 267–268.
- 18 H. G. Kunkel and A. Tiselius, *J. Gen. Physiol.*, 1951, **35**, 89–118.
- 19 H. Rheinboldt, *Die Methoden der Organischen Chemie*, Thieme Publishers, Leipzig, 3rd edn, 1925.
- 20 A. W. Martinez, S. T. Phillips, M. J. Butte and G. M. Whitesides, *Angew. Chem., Int. Ed.*, 2007, **46**, 1318–1320.

21 Z. Nie, C. A. Nijhuis, J. Gong, X. Chen, A. Kumachev, A. W. Martinez, M. Narovlyansky and G. M. Whitesides, *Lab Chip*, 2010, **10**, 477–483.

22 G. Aragay, J. Pons and A. Merkoçi, *Chem. Rev.*, 2011, **111**, 3433–3458.

23 V. Gubala, L. F. Harris, A. J. Ricco, M. X. Tan and D. E. Williams, *Anal. Chem.*, 2011, **84**, 487–515.

24 J. C. Jokerst, J. M. Emory and C. S. Henry, *Analyst*, 2012, **137**, 24–34.

25 X. Mao and T. J. Huang, *Lab Chip*, 2012, **12**, 1412–1416.

26 S. Nahavandi, S. Baratchi, R. Soffe, S.-Y. Tang, S. Nahavandi, A. Mitchell and K. Khoshmanesh, *Lab Chip*, 2014, **14**, 1496–1514.

27 E. K. Sackmann, A. L. Fulton and D. J. Beebe, *Nature*, 2014, **507**, 181–189.

28 A. W. Martinez, S. T. Phillips, G. M. Whitesides and E. Carrilho, *Anal. Chem.*, 2009, **82**, 3–10.

29 D. R. Ballerini, X. Li and W. Shen, *Microfluid. Nanofluid.*, 2012, **13**, 769–787.

30 D. D. Liana, B. Raguse, J. J. Gooding and E. Chow, *Sensors*, 2012, **12**, 11505–11526.

31 J. Nie, Y. Zhang, L. Lin, C. Zhou, S. Li, L. Zhang and J. Li, *Anal. Chem.*, 2012, **84**, 6331–6335.

32 W. K. Tomazelli Coltro, C. M. Cheng, E. Carrilho and D. P. Jesus, *Electrophoresis*, 2014, **35**, 2309–2324.

33 C. R. Mace and R. N. Deraney, *Microfluid. Nanofluid.*, 2014, **16**, 801–809.

34 D. M. Cate, J. A. Adkins, J. Mettakoonpitak and C. S. Henry, *Anal. Chem.*, 2015, **87**, 19–41.

35 Y. He, Y. Wu, J.-Z. Fu and W.-B. Wu, *RSC Adv.*, 2015, **5**, 78109–78127.

36 K. Yamada, T. G. Henares, K. Suzuki and D. Citterio, *Angew. Chem., Int. Ed.*, 2015, **54**, 5294–5310.

37 S. K. Mahadeva, K. Walus and B. Stoeber, *ACS Appl. Mater. Interfaces*, 2015, **7**, 8345–8362.

38 S. Ahmed, M.-P. N. Bui and A. Abbas, *Biosens. Bioelectron.*, 2016, **77**, 249–263.

39 R. Pelton, *TrAC, Trends Anal. Chem.*, 2009, **28**, 925–942.

40 F. Kong and Y. F. Hu, *Anal. Bioanal. Chem.*, 2012, **403**, 7–13.

41 E. W. Nery and L. T. Kubota, *Anal. Bioanal. Chem.*, 2013, **405**, 7573–7595.

42 A. K. Yetisen, M. S. Akram and C. R. Lowe, *Lab Chip*, 2013, **13**, 2210–2251.

43 C. Rozand, *Eur. J. Clin. Microbiol.*, 2014, **33**, 147–156.

44 J. Hu, S. Wang, L. Wang, F. Li, B. Pingguan-Murphy, T. J. Lu and F. Xu, *Biosens. Bioelectron.*, 2014, **54**, 585–597.

45 B. Liu, D. Du, X. Hua, X. Y. Yu and Y. Lin, *Electroanalysis*, 2014, **26**, 1214–1223.

46 J. Adkins, K. Boehle and C. Henry, *Electrophoresis*, 2015, **36**, 1811–1824.

47 S.-G. Jeong, J. Kim, J.-O. Nam, Y. S. Song and C.-S. Lee, *Int. Neurourol. J.*, 2013, **17**, 155–161.

48 P. Lisowski and P. K. Zarzycki, *Chromatographia*, 2013, **76**, 1201–1214.

49 G. Sun, K. Crissman, J. Norwood, J. Richards, R. Slade and G. E. Hatch, *Am. J. Physiol.: Lung Cell. Mol. Physiol.*, 2001, **281**, L807–L815.

50 K. L. Dreher, R. H. Jaskot, J. R. Lehmann, J. H. Richards, J. K. M. A. J. Ghio and D. L. Costa, *J. Toxicol. Environ. Health, Part A*, 1997, **50**, 285–305.

51 K. Jomova and M. Valko, *Toxicology*, 2011, **283**, 65–87.

52 R. Mehra and M. Juneja, *Indian J. Biochem. Biophys.*, 2004, **41**, 53–56.

53 J.-H. Lin, Z.-H. Wu and W.-L. Tseng, *Anal. Methods*, 2010, **2**, 1874–1879.

54 W. Pickering, *Ore Geol. Rev.*, 1986, **1**, 83–146.

55 M. M. Mentele, J. Cunningham, K. Koehler, J. Volckens and C. S. Henry, *Anal. Chem.*, 2012, **84**, 4474–4480.

56 P. Rattanarat, W. Dungchai, D. M. Cate, W. Siangproh, J. Volckens, O. Chailapakul and C. S. Henry, *Anal. Chim. Acta*, 2013, **800**, 50–55.

57 D. M. Cate, P. Nanthalasurasak, P. Riwkulkajorn, C. L'Orange, C. S. Henry and J. Volckens, *Ann. Occup. Hyg.*, 2014, **58**, 413–423.

58 M. I. G. Almeida, C. Chan, V. J. Pettigrove, R. W. Cattrall and S. D. Kolev, *Environ. Pollut.*, 2014, **193**, 233–239.

59 S. Chaiyo, W. Siangproh, A. Apilux and O. Chailapakul, *Anal. Chim. Acta*, 2015, **866**, 75–83.

60 S. Z. Hossain and J. D. Brennan, *Anal. Chem.*, 2011, **83**, 8772–8778.

61 B. M. Jayawardane, R. W. Cattrall and S. D. Kolev, *Anal. Chim. Acta*, 2013, **803**, 106–112.

62 M. Li, R. Cao, A. Nilghaz, L. Guan, X. Zhang and W. Shen, *Anal. Chem.*, 2015, **87**, 2555–2559.

63 A. Sadollahkhani, A. Hatamie, O. Nur, M. Willander, B. Zargar and I. Kazeminezhad, *ACS Appl. Mater. Interfaces*, 2014, **6**, 17694–17701.

64 Y. Zhang, C. Zhou, J. Nie, S. Le, Q. Qin, F. Liu, Y. Li and J. Li, *Anal. Chem.*, 2014, **86**, 2005–2012.

65 A. Apilux, W. Siangproh, N. Praphairaksit and O. Chailapakul, *Talanta*, 2012, **97**, 388–394.

66 N. Ratnarathorn, O. Chailapakul, C. S. Henry and W. Dungchai, *Talanta*, 2012, **99**, 552–557.

67 M. Elavarasi, A. Rajeshwari, N. Chandrasekaran and A. Mukherjee, *Anal. Methods*, 2013, **5**, 6211–6218.

68 D. M. Cate, W. Dungchai, J. C. Cunningham, J. Volckens and C. S. Henry, *Lab Chip*, 2013, **13**, 2397–2404.

69 D. M. Cate, S. D. Noblitt, J. Volckens and C. S. Henry, *Lab Chip*, 2015, **15**, 2808–2818.

70 L. Liu and H. Lin, *Anal. Chem.*, 2014, **86**, 8829–8834.

71 R. Patidar, B. Rebary and P. Paul, *J. Fluoresc.*, 2015, **25**, 387–395.

72 A. Apilux, W. Dungchai, W. Siangproh, N. Praphairaksit, C. S. Henry and O. Chailapakul, *Anal. Chem.*, 2010, **82**, 1727–1732.

73 P. Rattanarat, W. Dungchai, D. Cate, J. Volckens, O. Chailapakul and C. S. Henry, *Anal. Chem.*, 2014, **86**, 3555–3562.

74 World Health Organization, Cyanobacterial toxins, http://www.who.int/water_sanitation_health/diseases/cyanobacteria/en/, (accessed September, 2015).

75 K. G. Sellner, G. J. Doucette and G. J. Kirkpatrick, *J. Ind. Microbiol. Biotechnol.*, 2003, **30**, 383–406.

76 World Health Organization, Methaemoglobinemia, http://www.who.int/water_sanitation_health/diseases/methaemoglob/en/, (accessed September, 2015).

77 L. Fewtrell, *Environ. Health Perspect.*, 2004, **112**, 1371–1374.

78 World Health Organization, Fluorosis, http://www.who.int/water_sanitation_health/diseases/fluorosis/en/, (accessed September, 2015).

79 D. L. Ozsvath, *Rev. Environ. Sci. Biotechnol.*, 2009, **8**, 59–79.

80 United State Environmental Protection Agency, Cyanide compounds, <http://www3.epa.gov/ttn/atw/hlthef/cyanide.html>, (accessed January, 2016).

81 J. O. Egekeze and F. W. Oehme, *Vet. Q.*, 1980, **2**, 104–114.

82 B. M. Jayawardane, I. D. McKelvie and S. D. Kolev, *Talanta*, 2012, **100**, 454–460.

83 Q. He, C. Ma, X. Hu and H. Chen, *Anal. Chem.*, 2013, **85**, 1327–1331.

84 P. K. Kao and C. C. Hsu, *Anal. Chem.*, 2014, **86**, 8757–8762.

85 P.-K. Kao and C.-C. Hsu, *Microfluid. Nanofluid.*, 2014, **16**, 811–818.

86 B. Li, L. Fu, W. Zhang, W. Feng and L. Chen, *Electrophoresis*, 2014, **35**, 1152–1159.

87 C. H. Weng, M. Y. Chen, C. H. Shen and R. J. Yang, *Bio-microfluidics*, 2014, **8**, 066502.

88 N. Lopez-Ruiz, V. F. Curto, M. M. Erenas, F. Benito-Lopez, D. Diamond, A. J. Palma and L. F. Capitan-Vallvey, *Anal. Chem.*, 2014, **86**, 9554–9562.

89 B. M. Jayawardane, S. Wei, I. D. McKelvie and S. D. Kolev, *Anal. Chem.*, 2014, **86**, 7274–7279.

90 T. M. Cardoso, P. T. Garcia and W. K. Coltro, *Anal. Methods*, 2015, **7**, 7311–7317.

91 Y. He, W.-b. Wu and J.-z. Fu, *RSC Adv.*, 2015, **5**, 2694–2701.

92 Y. Chen, Y. Zilberman, P. Mostafalu and S. R. Sonkusale, *Biosens. Bioelectron.*, 2015, **67**, 477–484.

93 B. M. Jayawardane, I. D. McKelvie and S. D. Kolev, *Anal. Chem.*, 2015, **87**, 4621–4626.

94 P. Nath, R. K. Arun and N. Chanda, *RSC Adv.*, 2014, **4**, 59558–59561.

95 Y. Hao, W. Chen, L. Wang, B. Zhou, Q. Zang, S. Chen and Y.-N. Liu, *Anal. Methods*, 2014, **6**, 2478.

96 S. Karita and T. Kaneta, *Anal. Chem.*, 2014, **86**, 12108–12114.

97 M. Cuartero, G. A. Crespo and E. Bakker, *Anal. Chem.*, 2015, **87**, 1981–1990.

98 W. J. Lan, X. U. Zou, M. M. Hamed, J. Hu, C. Parolo, E. J. Maxwell, P. Buhlmann and G. M. Whitesides, *Anal. Chem.*, 2014, **86**, 9548–9553.

99 G. Lisak, J. Cui and J. Bobacka, *Sens. Actuators, B*, 2015, **207**, 933–939.

100 M. Novell, M. Parrilla, G. A. Crespo, F. X. Rius and F. J. Andrade, *Anal. Chem.*, 2012, **84**, 4695–4702.

101 K. C. Jones and P. De Voogt, *Environ. Pollut.*, 1999, **100**, 209–221.

102 A. Abelsohn, B. L. Gibson, M. D. Sanborn and E. Weir, *Can. Med. Assoc. J.*, 2002, **166**, 1549–1554.

103 M. El-Shahawi, A. Hamza, A. Bashammakh and W. Al-Saggaf, *Talanta*, 2010, **80**, 1587–1597.

104 D. Pardasani, V. Tak, A. K. Purohit and D. Dubey, *Analyst*, 2012, **137**, 5648–5653.

105 W. Y. Wei and I. M. White, *Analyst*, 2013, **138**, 1020–1025.

106 T. Eaidkong, R. Mungkarndee, C. Phollookin, G. Tumcharern, M. Sukwattanasinitt and S. Wacharasindhu, *J. Mater. Chem.*, 2012, **22**, 5970–5977.

107 K. A. Mirica, J. G. Weis, J. M. Schnorr, B. Esser and T. M. Swager, *Angew. Chem., Int. Ed.*, 2012, **51**, 10740–10745.

108 T. Soga, Y. Jimbo, K. Suzuki and D. Citterio, *Anal. Chem.*, 2013, **85**, 8973–8978.

109 B. Yoon, I. S. Park, H. Shin, H. J. Park, C. W. Lee and J. M. Kim, *Macromol. Rapid Commun.*, 2013, **34**, 731–735.

110 R. S. Alkasir, M. Ornatska and S. Andreeescu, *Anal. Chem.*, 2012, **84**, 9729–9737.

111 M. Santhiago, C. S. Henry and L. T. Kubota, *Electrochim. Acta*, 2014, **130**, 771–777.

112 G. Sun, P. Wang, S. Ge, L. Ge, J. Yu and M. Yan, *Biosens. Bioelectron.*, 2014, **56**, 97–103.

113 P. Tee-ngam, N. Nunant, P. Rattanarat, W. Siangproh and O. Chailapakul, *Sensors*, 2013, **13**, 13039–13053.

114 C. A. Staples, P. B. Dome, G. M. Klecka, S. T. Oblock and L. R. Harris, *Chemosphere*, 1998, **36**, 2149–2173.

115 W.-T. Tsai, *J. Environ. Sci. Health, Part C: Environ. Carcinog. Ecotoxicol. Rev.*, 2006, **24**, 225–255.

116 M. S. Golub, K. L. Wu, F. L. Kaufman, L. H. Li, F. Moran-Messen, L. Zeise, G. V. Alexeef and J. M. Donald, *Birth Defects Res., Part B*, 2010, **89**, 441–466.

117 S. Flint, T. Markle, S. Thompson and E. Wallace, *J. Environ. Manage.*, 2012, **104**, 19–34.

118 R. S. Alkasir, A. Rossner and S. Andreeescu, *Environ. Sci. Technol.*, 2015, **49**, 9889–9897.

119 L. J. Casarett, C. D. Klaassen and M. O. Amdur, *Casarett and Doull's Toxicology: The Basic Science of Poisons*, McGraw-Hill, New York, 7th edn, 2008.

120 B. Binukumar, A. Bal, A. Sunkaria and K. D. Gill, *Toxicology*, 2010, **270**, 77–84.

121 Z. Xu, G. Fang and S. Wang, *Food Chem.*, 2010, **119**, 845–850.

122 T. Duarte, C. Martin, F. J. Baud, O. Laprévote and P. Houzé, *Toxicol. Lett.*, 2012, **213**, 142–150.

123 Z. Zheng, Y. Zhou, X. Li, S. Liu and Z. Tang, *Biosens. Bioelectron.*, 2011, **26**, 3081–3085.

124 M. Pohanka, *Anal. Lett.*, 2012, **45**, 367–374.

125 S. Z. Hossain, R. E. Luckham, A. M. Smith, J. M. Lebert, L. M. Davies, R. H. Pelton, C. D. Filipe and J. D. Brennan, *Anal. Chem.*, 2009, **81**, 5474–5483.

126 J. S. Van Dyk and B. Pletschke, *Chemosphere*, 2011, **82**, 291–307.

127 H. Liang and M. T. Hay, *Water Environ. Res.*, 2011, **83**, 956–982.

128 F. Arduini and A. Amine, in *Biosensors Based on Aptamers and Enzymes*, Springer, 2014, pp. 299–326.

129 W. Liu, J. Kou, H. Xing and B. Li, *Biosens. Bioelectron.*, 2014, **52**, 76–81.

130 S. Wang, L. Ge, L. Li, M. Yan, S. Ge and J. Yu, *Biosens. Bioelectron.*, 2013, **50**, 262–268.

131 M. Pohanka, M. Hrabinova, J. Fusek, D. Hynek, V. Adam, J. Hubalek and R. Kizek, *Int. J. Electrochem. Sci.*, 2012, **7**, 50–57.

132 M. E. Badawy and A. F. El-Aswad, *Int. J. Anal. Chem.*, 2014, 2014.

133 C. Sicard, C. Glen, B. Aubie, D. Wallace, S. Jahanshahi-Anbuhi, K. Pennings, G. T. Daigger, R. Pelton, J. D. Brennan and C. D. M. Filipe, *Water Res.*, 2015, **70**, 360–369.

134 M. Pohanka, J. Z. Karasova, K. Kuca, J. Pikula, O. Holas, J. Korabecny and J. Cabal, *Talanta*, 2010, **81**, 621–624.

135 Y. Su, S. Ma, K. Jiang and X. Han, *Chin. J. Chem.*, 2015, **33**, 446–450.

136 R. Pimsen, A. Khumsri, S. Wacharasindhu, G. Tumcharern and M. Sukwattanasinitt, *Biosens. Bioelectron.*, 2014, **62**, 8–12.

137 W. Liu, Y. Guo, J. Luo, J. Kou, H. Zheng, B. Li and Z. Zhang, *Spectrochim. Acta, Part A*, 2015, **141**, 51–57.

138 S. Z. Hossain, R. E. Luckham, M. J. McFadden and J. D. Brennan, *Anal. Chem.*, 2009, **81**, 9055–9064.

139 S. Burnham, J. Hu, H. Anany, L. Brovko, F. Deiss, R. Derda and M. W. Griffiths, *Anal. Bioanal. Chem.*, 2014, **406**, 5685–5693.

140 S. Z. Hossain, C. Ozimok, C. Sicard, S. D. Aguirre, M. M. Ali, Y. Li and J. D. Brennan, *Anal. Bioanal. Chem.*, 2012, **403**, 1567–1576.

141 J. C. Jokerst, J. A. Adkins, B. Bisha, M. M. Mentele, L. D. Goodridge and C. S. Henry, *Anal. Chem.*, 2012, **84**, 2900–2907.

142 H. Liu, F. Zhan, F. Liu, M. Zhu, X. Zhou and D. Xing, *Biosens. Bioelectron.*, 2014, **62**, 38–46.

143 S. Ma, Y. Tang, J. Liu and J. Wu, *Talanta*, 2014, **120**, 135–140.

144 F. Liu and C. Zhang, *Sens. Actuators, B*, 2015, **209**, 399–406.

145 T. San Park, W. Li, K. E. McCracken and J.-Y. Yoon, *Lab Chip*, 2013, **13**, 4832–4840.

146 B. Bisha, J. A. Adkins, J. C. Jokerst, J. C. Chandler, A. Perez-Mendez, S. M. Coleman, A. O. Sbodio, T. V. Suslow, M. D. Danyluk and C. S. Henry, *J. Visualized Exp.*, 2014, e51414.

147 R. V. Taudte, A. Beavis, L. Wilson-Wilde, C. Roux, P. Doble and L. Blanes, *Lab Chip*, 2013, **13**, 4164–4172.

148 J. Szram, S. J. Schofield, M. P. Cosgrove and P. Cullinan, *Eur. Respir. J.*, 2013, **42**, 1186–1193.

149 A. Pesenti, R. V. Taudte, B. McCord, P. Doble, C. Roux and L. Blanes, *Anal. Chem.*, 2014, **86**, 4707–4714.

150 K. L. Peters, I. Corbin, L. M. Kaufman, K. Zreibé, L. Blanes and B. R. McCord, *Anal. Methods*, 2015, **7**, 63–70.

151 M. Salles, G. Meloni, W. de Araujo and T. Paixão, *Anal. Methods*, 2014, **6**, 2047–2052.

152 M. Xu, B. R. Bunes and L. Zang, *ACS Appl. Mater. Interfaces*, 2011, **3**, 642–647.

153 P. M. Fierro-Mercado and S. P. Hernández-Rivera, *Int. J. Spectrosc.*, 2012, **2012**, 716527.

154 T. Finkel and N. J. Holbrook, *Nature*, 2000, **408**, 239–247.

155 N. Li, C. Sioutas, A. Cho, D. Schmitz, C. Misra, J. Sempf, M. Wang, T. Oberley, J. Froines and A. Nel, *Environ. Health Perspect.*, 2003, **111**, 455–460.

156 P. Møller, J. K. Folkmann, L. Forchhammer, E. V. Bräuner, P. H. Danielsen, L. Risom and S. Loft, *Cancer Lett.*, 2008, **266**, 84–97.

157 L. Risom, P. Møller and S. Loft, *Mutat. Res., Fundam. Mol. Mech. Mutagen.*, 2005, **592**, 119–137.

158 V. Mani, K. Kadimisetty, S. Malla, A. A. Joshi and J. F. Rusling, *Environ. Sci. Technol.*, 2013, **47**, 1937–1944.

159 A. Eiguren-Fernandez, E. Di Stefano, D. A. Schmitz, A. L. N. Guarieiro, E. M. Salinas, E. Nasser, J. R. Froines and A. K. Cho, *J. Air Waste Manage. Assoc.*, 2015, **65**, 270–277.

160 K. A. Koehler, J. Shapiro, Y. Sameenoi, C. Henry and J. Volckens, *Aerosol Sci. Technol.*, 2014, **48**, 489–497.

161 Y. Sameenoi, K. Koehler, J. Shapiro, K. Boonsong, Y. Sun, J. Collett Jr., J. Volckens and C. S. Henry, *J. Am. Chem. Soc.*, 2012, **134**, 10562–10568.

162 Y. Sameenoi, P. Panymeesamer, N. Supalakorn, K. Koehler, O. Chailapakul, C. S. Henry and J. Volckens, *Environ. Sci. Technol.*, 2012, **47**, 932–940.

163 F. Ciriello, M. Gualtieri, E. Longhin, R. Ruffo, M. Camatini and P. Parenti, *Environ. Sci. Pollut. Res.*, 2015, **22**, 12469–12478.

164 W. Dungchai, Y. Sameenoi, O. Chailapakul, J. Volckens and C. S. Henry, *Analyst*, 2013, **138**, 6766–6773.

165 N. R. Pollock, J. P. Rolland, S. Kumar, P. D. Beattie, S. Jain, F. Noubary, V. L. Wong, R. A. Pohlmann, U. S. Ryan and G. M. Whitesides, *Sci. Transl. Med.*, 2012, **4**, 152ra129–152ra129.

166 A. K. Yetisen, J. Martinez-Hurtado, A. Garcia-Melendrez, F. da Cruz Vasconcellos and C. R. Lowe, *Sens. Actuators, B*, 2014, **196**, 156–160.

167 G. G. Lewis, M. J. DiTucci and S. T. Phillips, *Angew. Chem., Int. Ed.*, 2012, **124**, 12879–12882.

168 G. G. Lewis, J. S. Robbins and S. T. Phillips, *Anal. Chem.*, 2013, **85**, 10432–10439.

169 G. G. Lewis, J. S. Robbins and S. T. Phillips, *Chem. Commun.*, 2014, **50**, 5352–5354.

170 A. A. Rowe, A. J. Bonham, R. J. White, M. P. Zimmer, R. J. Yadgar, T. M. Hobza, J. W. Honea, I. Ben-Yaacov and K. W. Plaxco, *PLoS One*, 2011, **6**, e23783.

171 A. Nemirovski, D. C. Christodouleas, J. W. Hennek, A. A. Kumar, E. J. Maxwell, M. T. Fernández-Abedul and G. M. Whitesides, *Proc. Natl. Acad. Sci. U. S. A.*, 2014, **111**, 11984–11989.

172 I. Ramfos, N. Vassiliadis, S. Blionas, K. Efstathiou, A. Fragoso, C. K. O'Sullivan and A. Birbas, *Biosens. Bioelectron.*, 2013, **47**, 482–489.

173 W. K. Coltro, M. F. Mora, C. D. Garcia, A. Escarpa, M. C. González and M. Á. López, *Agricultural and Food Electroanalysis*, 2015, pp. 443–477.

174 B.-Y. Chang, *Bull. Korean Chem. Soc.*, 2012, **33**, 549–552.

175 J. L. Delaney, E. H. Doeven, A. J. Harsant and C. F. Hogan, *Anal. Chim. Acta*, 2013, **790**, 56–60.

176 C. F. Fronczek, T. San Park, D. K. Harshman, A. M. Nicolini and J.-Y. Yoon, *RSC Adv.*, 2014, **4**, 11103–11110.

177 A. W. Martinez, S. T. Phillips, E. Carrilho, S. W. Thomas III, H. Sindi and G. M. Whitesides, *Anal. Chem.*, 2008, **80**, 3699–3707.

178 O. Mudanyali, S. Dimitrov, U. Sikora, S. Padmanabhan, I. Navruz and A. Ozcan, *Lab Chip*, 2012, **12**, 2678–2686.

179 X. Li, D. R. Ballerini and W. Shen, *Biomicrofluidics*, 2012, **6**, 11301–1130113.

180 N. K. Thom, G. G. Lewis, K. Yeung and S. T. Phillips, *RSC Adv.*, 2014, **4**, 1334–1340.

181 N. K. Thom, K. Yeung, M. B. Pillion and S. T. Phillips, *Lab Chip*, 2012, **12**, 1768–1770.

182 H. Wang, Y.-j. Li, J.-f. Wei, J.-r. Xu, Y.-h. Wang and G.-x. Zheng, *Anal. Bioanal. Chem.*, 2014, **406**, 2799–2807.

183 N. M. Myers, E. N. Kernisan and M. Lieberman, *Anal. Chem.*, 2015, **87**, 3764–3770.

184 World Health Organization, Water-related diseases: information sheets, http://www.who.int/water_sanitation_health/diseases/diseasefact/en/, (accessed September, 2015).

185 United States Environmental Protection Agency, Drinking water contaminants, <http://water.epa.gov/drink/contaminants/>, (accessed September, 2015).

186 United States Environmental Protection Agency, Air pollutants, <http://www.epa.gov/air/airpollutants.html>, (accessed September, 2015).

187 United States Environmental Protection Agency, Nutrient pollution policy and data, <http://www2.epa.gov/nutrient-policy-data>, (accessed September, 2015).

188 Centers for Disease Control and Prevention, NIOSH pocket guide to chemical hazards, <http://www.cdc.gov/niosh/npg/>, (accessed January, 2016).

189 United States Environmental Protection Agency, Table of regulated drinking water contaminants, <http://www.epa.gov/your-drinking-water/table-regulated-drinking-water-contaminants>, (accessed January, 2016).