



HHS Public Access

Author manuscript

J Vis Exp. Author manuscript; available in PMC 2014 August 21.

Published in final edited form as:

J Vis Exp. ; (84): e51510. doi:10.3791/51510.

Lipid Bilayer Vesicle Generation Using Microfluidic Jetting

Christopher W. Coyne,

Department of Mechanical Engineering, University of Michigan, Ann Arbor, MI USA

Karan Patel,

Department of Mechanical Engineering, University of Michigan, Ann Arbor, MI USA

Johanna Heureaux,

Department of Mechanical Engineering, University of Michigan, Ann Arbor, MI USA

Jeanne Stachowiak,

Department of Biomedical Engineering, Institute for Cellular and Molecular Biology, The University of Texas at Austin, Austin, Texas USA

Daniel A. Fletcher, and

Department of Bioengineering, University of California, Berkeley, Lawrence Berkeley National Laboratory, Physical Biosciences Division, Berkeley, CA USA

Allen P. Liu

Department of Mechanical Engineering, Department of Biomedical Engineering, Cellular and Molecular Biology Program, Biophysics Program, University of Michigan, Ann Arbor, MI USA

Christopher W. Coyne: ccoyne@umich.edu; Karan Patel: karanp@umich.edu; Johanna Heureaux: heureaux@umich.edu; Jeanne Stachowiak: jstach@austin.utexas.edu; Daniel A. Fletcher: fletch@berkeley.edu; Allen P. Liu: allenliu@umich.edu

Abstract

SHORT ABSTRACT—Microfluidic jetting against a droplet interface lipid bilayer provides a reliable way to generate vesicles with control over membrane asymmetry, incorporation of transmembrane proteins, and encapsulation of material. This technique can be applied to study a variety of biological systems where compartmentalized biomolecules are desired.

LONG ABSTRACT—Bottom-up synthetic biology presents a novel approach for investigating and reconstituting biochemical systems and, potentially, minimal organisms. This emerging field engages engineers, chemists, biologists, and physicists to design and assemble basic biological components into complex, functioning systems from the bottom up. Such bottom-up systems could lead to the development of artificial cells for fundamental biological inquiries and innovative therapies^{1,2}. Giant unilamellar vesicles (GUVs) can serve as a model platform for synthetic biology due to their cell-like membrane structure and size. Microfluidic jetting, or microjetting, is a technique that allows for the generation of GUVs with controlled size,

CORRESPONDING AUTHOR: Liu, Allen P., Department of Mechanical Engineering, Department of Biomedical Engineering, Cellular and Molecular Biology Program, Biophysics Program, University of Michigan, Ann Arbor, MI USA, allenliu@umich.edu.

A complete version of this article that includes the video component is available at <http://dx.doi.org/10.3791/51510>.

DISCLOSURES:

No conflicts of interest declared.

membrane composition, transmembrane protein incorporation, and encapsulation³. The basic principle of this method is the use of multiple, high-frequency fluid pulses generated by a piezo-actuated inkjet device to deform a suspended lipid bilayer into a GUV. The process is akin to blowing soap bubbles from a soap film. By varying the composition of the jetted solution, the composition of the encompassing solution, and/or the components included in the bilayer, researchers can apply this technique to create customized vesicles. This paper describes the procedure to generate simple vesicles from a droplet interface bilayer by microjetting.

Keywords

Microfluidic jetting; synthetic biology; vesicle encapsulation; lipid bilayer

INTRODUCTION

It has become increasingly clear that cell biology is a multi-scale problem that involves integrating our understanding from molecules to cells. Consequently, knowing precisely how molecules work individually is not sufficient to understand complex cellular behaviors. This is partly due to the existence of emergent behaviors of multi-component systems, as exemplified by the reconstitution of actin network interaction with lipid bilayer vesicles⁴, mitotic spindle assembly in *Xenopus* extract⁵, and spatial dynamics of bacterial cell division machineries⁶. One way to complement the reductionist's approach of dissecting the molecular processes of living systems is to take the opposite approach of reconstituting cellular behaviors using a minimal set of biological components. A critical part of this approach involves the reliable encapsulation of biomolecules in a confined volume, a key feature of a cell.

Several strategies exist for encapsulating biomolecules for studying biomimetic systems. The most biologically relevant system is lipid bilayer membranes, which mimic the biochemical and physical constraints imposed by the cell's plasma membrane. Formation of giant unilamellar vesicles (GUVs) by electroformation⁷, one of the most widely used techniques for GUV generation, typically has a poor encapsulation yield due to its incompatibility with high salt buffer⁸. Electroformation also requires larger sample volumes (>100 μ l), which could be a problem for working with purified proteins, and inefficiently incorporates large molecules due to difficulty of diffusion between closely spaced lipid layers. Several microfluidic approaches for generating lipid vesicles have been developed. The double emulsion methods, which pass components through two interfaces between layers water-oil-water (W/O/W), relies on the evaporation of a volatile solvent to drive lipid bilayer formation⁹. Others have used a microfluidic assembly line that produces a continuous stream of lipid bilayer vesicles¹⁰ or in two independent steps¹¹. We have developed an alternate technique based on rapidly applying fluid pulses against a droplet interface bilayer¹² to produce GUVs of controlled size, composition, and encapsulation. Our approach, known as microfluidic jetting, offers the combined advantages from several existing vesicle generation techniques, providing an approach for creating functional biomolecular systems for investigating a variety of biological problems.

PROTOCOL

1. Infinity Chamber Fabrication

- 1.1) Design the infinity chamber (name based on the shape of the chamber) (called that because of its shape) using a computer assisted design (CAD) software, and save the file such that it is compatible with a laser cutter. The design used was created by separating two circles of diameter 0.183" by a center-to-center distance of 0.15". The infinity shape facilitates droplet interface bilayer formation and stability. Cut the chamber from 1/8" – 3/16" clear acrylic with the laser cutter.
- 1.2) Drill a 1/16" hole through the edge of the acrylic chamber to the infinity-shaped well. Repeat on the opposite side.
- 1.3) Cut a small rectangle from a 0.2 mm acrylic sheet with scissors or a laser cutter to serve as a bottom to the wells.
- 1.4) Apply a thin but thorough layer of quick-drying adhesive to one side of the 0.2 mm acrylic and glue it to the bottom of the chamber. Holding the 0.2 mm acrylic tightly in place against the bottom of the chamber and dispensing the glue at the interface will allow the glue to create a seal but avoid covering the viewing area. Be sure to align the acrylic so that its edge is flush with the edge of the chamber wall and it completely covers the infinity chamber cutout. This will allow for sufficient jet penetration and prevent leakage of the well.
- 1.5) Cut two small pieces of natural rubber to cover the drilled holes.
- 1.6) Apply quick-drying adhesive around the hole. Place the rubber over the hole and press on all areas with a pair of forceps to secure. Repeat for both drilled holes. Be sure that all glued connections are complete seals so as to prevent any leakage.
- 1.7) Poke a hole in the natural rubber on both sides of the chamber to facilitate insertion of the piezoelectric inkjet tip. This can be done with a 23G, 1" needle.

2. Experimental Preparation

- 2.1) Stock lipid solution in chloroform is stored in a –20 °C freezer. For this study, either 1,2-diphytanoyl-*sn*-glycero-3-phosphocholine (DPhPC) or 1,2-dioleoyl-*sn*-glycero-3-phosphocholine (DOPC) was used. To resuspend the lipid in *n*-decane, first transfer it from a stock vial to a small glass jar, and gently dry under argon or nitrogen. Holding the jar at an angle while drying exposes more surface area to the gas, which allows the lipid to dry faster.
- 2.2) With the cap of the jar only slightly screwed on, allow the dried solution to sit under vacuum in a desiccator for 1–2 hrs Then add *n*-decane to resolubilize the lipid at 25 mg/ml. Vortex the lipid solution briefly and sonicate in a bath sonicator for 15 min. The reconstituted lipid in *n*-decane is stored at –20 °C.

- 2.3) Prepare a stock sucrose solution. A 300 mOsm sucrose solution is prepared in this protocol to match cellular osmolarity and to provide contrast during microjetting. In a 1.5 ml microcentrifuge tube, add 900 μ l of sucrose and 100 μ l of 1% methylcellulose (MC). An optional 1 μ l of dark-colored food dye or fluorescent beads can be added to lend more contrast or fluorescence in imaging, respectively.
- 2.4) Draw the solution into a disposable 1 ml plastic syringe. While holding the syringe with the tip facing upwards, flick the shaft repeatedly to expel any bubbles toward the tip, and push the plunger to eject the trapped air. Be sure to evacuate all air from the syringe before proceeding, as it will interfere with proper piezoelectric contraction responsible for jetting.
- 2.5) Install a 0.22 μ m filter on the end of the syringe. A 33 mm diameter syringe filter unit was found to work best, but alternative filters as small as a 3 mm diameter syringe filter can be used to reduce dead volume. To prevent air from being trapped in the filter, hold the syringe vertically and push the plunger until a droplet is formed above the tip.
- 2.6) Unscrew the female Luer adapter of the inkjet, and securely press it in place over the end of the filter. Again, eject fluid to prevent trapping air.
- 2.7) Screw in the top of the inkjet. Fluid should travel to the tip of the inkjet after it is completely attached.

3. Readyng the Equipment

- 3.1) Using a v-clamp, mount the syringe assembly on the microscope stage. A custom stage was built for this protocol; while the stage design can be determined by the user, it is critical to have independent x-y-z control of the syringe and x-y control of the sample holder. Additionally, attach the wire from the inkjet to the inkjet controller.
- 3.2) Determine the magnification and necessary lens combination to achieve the desired imaging. A 10X objective and 10X eyepiece were used throughout this protocol.
- 3.3) Use a high-speed camera (1000 fps) in order to visualize the jetting and vesicle generation.
- 3.4) Prior to imaging, perform necessary camera calibration. For this protocol, image-based auto-trigger within the camera software was used to initiate image capture.
- 3.5) Mount the infinity chamber onto the microscope stage. Secure the chamber by taping it into place on the stage.
- 3.6) Carefully align the inkjet tip with the hole punctured in the natural rubber (see Fig. 1b). It is best to bring the inkjet close to the chamber and adjust the positioning by eye, then make more precise adjustments through the microscope lens.

- 3.7) Once the inkjet is aligned, back the syringe assembly away from the chamber to prevent any damage to the inkjet during loading of the wells. Be sure that motion of the inkjet is unidirectional so that it remains aligned with the hole in the membrane.
- 3.8) Press gently on plunger of the syringe assembly until a small droplet forms at the inkjet nozzle. This will provide some initial backpressure.
- 3.9) Input the jetting parameters. Assuming a trapezoidal bipolar wave is used, parameters that are generally consistent across trials include: 20 kHz pulse frequency, 3 μ s rise time, 35 μ s pulse duration, and 3 μ s fall time. Variable parameters include applied voltage (pulse amplitude) and pulse number (jet pulses per trigger).

4. Vesicle Generation

- 4.1) Add 25–30 μ l lipid solution suspended in *n*-decane, covering the full surface of both wells.
- 4.2) Add 25 μ l glucose (of same osmolarity as the sucrose solution) to the outermost edge of each well, pipetting slowly and smoothly. Upon the first addition, a drop of glucose should form, because the glucose and lipid solution do not mix. The second 25 μ l of glucose will make another drop and form the lipid bilayer membrane in the middle of the chamber within 5–10 min.
- 4.3) Insert the inkjet through the natural rubber, and carefully guide it towards the droplet interface bilayer. Approach the bilayer slowly, as the introduced inkjet will displace volume and can rupture the bilayer.
- 4.4) When the inkjet is within \sim 200 μ m, apply the jetting with the desired settings. The distance from the bilayer may vary primarily depending on the voltage and pulse number, among other parameters. This protocol recommends slowly increasing settings (voltage and pulse number) and observing bilayer deformation.

5. Cleaning the Equipment

- 5.1) Detach the syringe assembly from the microscope stage, and dispose of the 1 ml plastic syringe and filter.
- 5.2) To clean the inkjet, aspirate the following solutions in order by dipping the tip in the solution 7–10 times each: 70% ethanol, 2% Neutrad solution in warm water, 70% ethanol, and ddH₂O. If the inkjet doesn't fit securely on the aspiration pipette, cut a pipette tip to form an adapter.
- 5.3) Dry the chamber with tissue. Place the infinity chamber in a 250 ml beaker with 2% Neutrad in warm water, and sonicate for 5–10 min. After sonication, thoroughly dry the wells under compressed air. Any moisture in the wells can compromise the stability of the lipid bilayer membrane, so it is also recommended that the chambers are placed in an oven at 60 °C for 15 min.

REPRESENTATIVE RESULTS

We have assembled a microfluidic jetting setup on a conventional inverted fluorescence microscope with a custom stage assembled from machined parts and manual micrometers (Figure 1). Characterization of the inkjet provides insight into the vesicle generation process. Varying the distance between the inkjet nozzle and lipid bilayer affects the force applied to cause deformation of the membrane. Close proximity to the bilayer focuses the jet stream and prevents the membrane from dispersing energy away from the point of vesicle generation. The vortex travel increases with the voltage applied to the piezoelectric actuator, consistent with our expectation (Figure 2). Vesicle formation and representative jetted vesicles are shown in Figure 3. Figure 3a shows a representative image sequence for vesicle formation by microjetting. Following formation, vesicle stability tends to vary with vesicle diameter, where smaller vesicles were more stable.

DISCUSSION

Many techniques have been developed for vesicle generation, including electroformation, emulsion, and droplet generation¹⁴⁻¹⁶. However, new experimental techniques are necessary to allow for the design of biological systems with growing similarity to living systems. Microfluidic methods in particular have offered an increased level of control governing membrane unilamellarity, monodispersity of size, and internal contents^{17,18}, bringing vesicle models closer to biology. Furthermore, characterization and experimentation using microfluidic jetting has shown effective incorporation of oriented membrane proteins, membrane asymmetry, and encapsulation^{3,13}.

Vesicle generation by microfluidic jetting is reliable and repeatable; however, discrepancies amongst inkjets require some familiarity and parameterization. In our experience, the introduction of the inkjet nozzle into the infinity chamber prior to jetting may displace up to several microliters of glucose depending on the nozzle dimensions, producing a slight bend in the bilayer away from the inkjet. By disproportionately dispersing the glucose solution when originally establishing the bilayer, this effect can be offset and a planar bilayer will result. This not only enhances bilayer stability but also allows for better control over vesicle formation. Minimization of vibrations is also recommended; simple rubber cutouts were used to support the microscope table and dampen laboratory vibrations.

Although this protocol is applicable to many lipids, DPhPC was chosen for its particular chemical and high bilayer stability. Other primary lipids tested were 1,2-dipalmitoyl-*sn*-glycero-3-phosphocholine (DPPC) and 1,2-dioleoyl-*sn*-glycero-3-phosphocholine (DOPC). Comparatively, DPhPC had a stronger tendency to form a consistent bilayer that gradually grew thinner over time, and to produce unilamellar vesicles. This effect was tested under variability of the length of the bilayer; the initial chamber design was adjusted slightly (the second generation design consisted of two circles of diameter 0.015" separated by a center-to-center distance of 0.13") to necessitate smaller volumes and resulted in a smaller bilayer interface. Both the new and initial design allowed for accurate vesicle generation, yet neither design showed a dominant advantage in bilayer thinning. Another tested optimization was computer-controlled backpressure applied to the piezoelectric inkjet. While this gave a more

quantitative control over the flow rate while jetting, it was not used throughout the majority of experimentation.

This method offers the combined advantages of several existing techniques. Multiple GUVs can be generated at high frequency (~200 Hz) due to the high concentration of lipid molecules, although rapid vesicle generation was not the focus of this work. Since this technique jets against a single lipid bilayer, membrane unilamellarity is expected and has been observed. Additionally, a wide range of solutions can be encapsulated independent of specific solute properties such as molecular weight or charge, thus enabling more potential applications¹⁷. Also, due to the size of vesicles formed (a range is possible of <10 μm to >400 μm), observation by conventional microscopy techniques is adequate¹³.

Microfluidic jetting can be applied to a variety of biological problems. One specific example is cellular biomechanics; the deformability of GUVs renders them an ideal tool to study the force generation and self assembly of encapsulated actin networks that showed interesting effects when assembled on the surface of a GUV^{4,19}. Additional applications include drug delivery systems, cell-size bioreactors, modular systems for synthetic biology, biophysics, and a variety of other fields in basic science, industry, and medicine where compartmentalized biomolecules are desired.

Acknowledgments

We thank Mike Vahey from the Fletcher Lab at the University of California, Berkeley for advice on the microjetting parameters. This work was sponsored by NIH grant DP2 HL117748-01.

References

1. Liu AP, Fletcher DA. Biology under construction: in vitro reconstitution of cellular function. *Nature reviews. Molecular cell biology*. 2009; 10:644–650.10.1038/nrm2746
2. Yeh BJ, Lim WA. Synthetic biology: lessons from the history of synthetic organic chemistry. *Nature chemical biology*. 2007; 3:521–525.10.1038/nchembio0907-521
3. Richmond DL, et al. Forming giant vesicles with controlled membrane composition, asymmetry, and contents. *Proceedings of the National Academy of Sciences of the United States of America*. 2011; 108:9431–9436.10.1073/pnas.1016410108 [PubMed: 21593410]
4. Liu AP, et al. Membrane-induced bundling of actin filaments. *Nature physics*. 2008; 4:789–793.10.1038/nphys1071
5. Brown KS, et al. *Xenopus tropicalis* egg extracts provide insight into scaling of the mitotic spindle. *J Cell Biol*. 2007; 176:765–770.10.1083/jcb.200610043 [PubMed: 17339377]
6. Loose M, Fischer-Friedrich E, Ries J, Kruse K, Schwille P. Spatial regulators for bacterial cell division self-organize into surface waves in vitro. *Science*. 2008; 320:789–792.10.1126/science.1154413 [PubMed: 18467587]
7. Angelova MI, Dimitrov DS. Liposome electroformation. *Faraday Discussion of the Chemical Society*. 1986; 81:301–311.
8. Bucher P, Fischer A, Luisi LP, Oberholzer T, Walde P. Giant Vesicles as Biochemical Compartments: The Use of Microinjection Techniques. *Langmuir*. 1998; 14:2712–2721.10.1021/la971318g
9. Shum HC, Lee D, Yoon I, Kodger T, Weitz DA. Double emulsion templated monodisperse phospholipid vesicles. *Langmuir*. 2008; 24:7651–7653.10.1021/la801833a [PubMed: 18613709]
10. Matosevic S, Paegel BM. Stepwise Synthesis of Giant Unilamellar Vesicles on a Microfluidic Assembly Line. *Journal of the American Chemical Society*. 2011; 133:2798–2800.10.1021/Ja109137s [PubMed: 21309555]

11. Hu PCC, Li S, Malmstadt N. Microfluidic Fabrication of Asymmetric Giant Lipid Vesicles. *ACS Appl Mater Inter.* 2011; 3:1434–1440.10.1021/Am101191d
12. Hwang WL, Chen M, Cronin B, Holden MA, Bayley H. Asymmetric droplet interface bilayers. *Journal of the American Chemical Society.* 2008; 130:5878–5879.10.1021/ja802089s [PubMed: 18407631]
13. Stachowiak JC, Richmond DL, Li TH, Brochard-Wyart F, Fletcher DA. Inkjet formation of unilamellar lipid vesicles for cell-like encapsulation. *Lab on a chip.* 2009; 9:2003–2009.10.1039/b904984c [PubMed: 19568667]
14. Meleard P, Bagatolli LA, Pott T. Giant unilamellar vesicle electroformation from lipid mixtures to native membranes under physiological conditions. *Methods in enzymology.* 2009; 465:161–176.10.1016/S0076-6879(09)65009-6 [PubMed: 19913167]
15. Nishimura K, Suzuki H, Toyota T, Yomo T. Size control of giant unilamellar vesicles prepared from inverted emulsion droplets. *Journal of colloid and interface science.* 2012; 376:119–125.10.1016/j.jcis.2012.02.029 [PubMed: 22444482]
16. Teh SY, Lin R, Hung LH, Lee AP. Droplet microfluidics. *Lab on a chip.* 2008; 8:198–220.10.1039/b715524g [PubMed: 18231657]
17. Stachowiak JC, et al. Unilamellar vesicle formation and encapsulation by microfluidic jetting. *Proceedings of the National Academy of Sciences of the United States of America.* 2008; 105:4697–4702.10.1073/pnas.0710875105 [PubMed: 18353990]
18. Osaki T, Yoshizawa S, Kawano R, Sasaki H, Takeuchi S. Lipid-coated microdroplet array for in vitro protein synthesis. *Analytical chemistry.* 2011; 83:3186–3191.10.1021/ac2000048 [PubMed: 21417316]
19. Liu AP, Fletcher DA. Actin polymerization serves as a membrane domain switch in model lipid bilayers. *Biophysical journal.* 2006; 91:4064–4070.10.1529/biophysj.106.090852 [PubMed: 16963509]

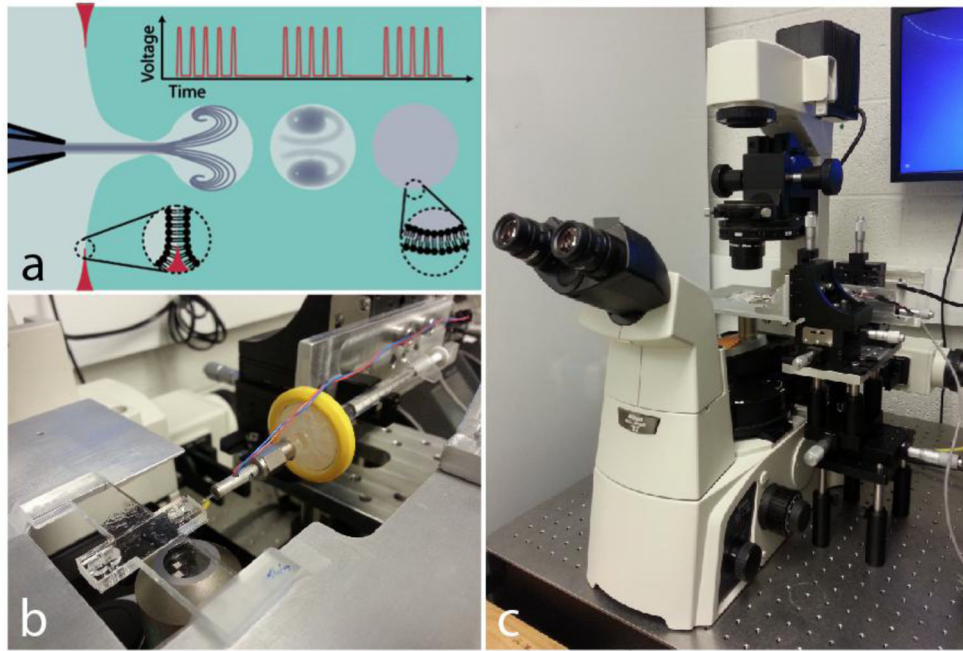


Figure 1. Illustration of the technique and equipment. (a) Schematic of piezoelectric-driven jetting process against the droplet interface bilayer. Multiple pulses pushed out in rapid succession form a vortex ring structure that deforms the bilayer to produce GUVs (image adopted from Stachowiak *et al.*¹³). (b) The mounted syringe assembly, custom holding platform, and infinity chamber. The chamber is secured in place, and the tip of the inkjet is aligned with the hole in the natural rubber on the side of the well. (c) The complete microscope and custom stage assembly.

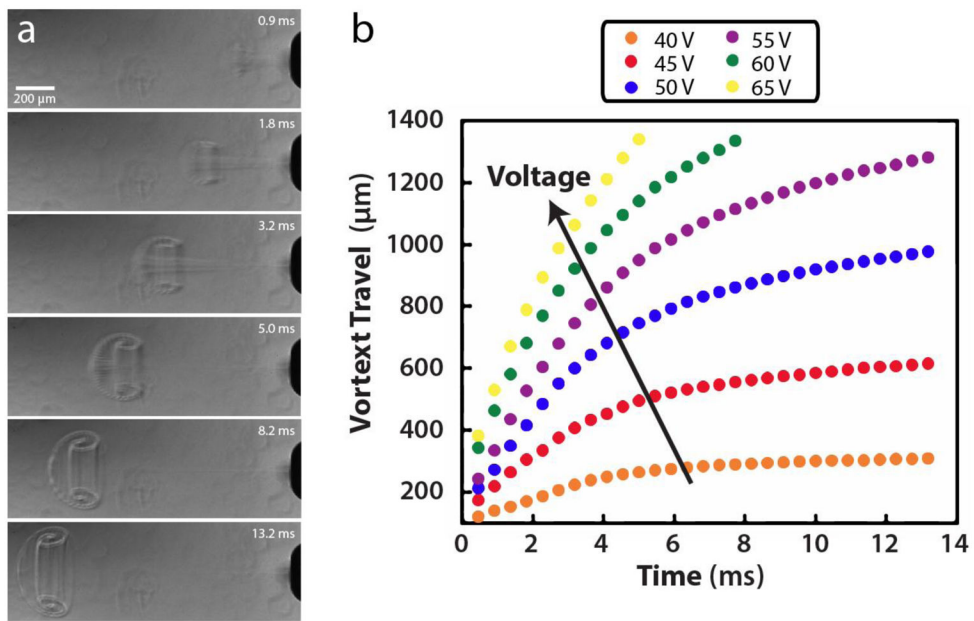


Figure 2. Characterization of the Inkjet. (a) Rapid inkjet pulses at 20 kHz (50 pulses at 55V pulse amplitude) overlap to form a single vortex ring. (b) Liquid jet front displacement as a function of time over pulse amplitude range (40V-65V) for fixed pulse number (200 pulses).

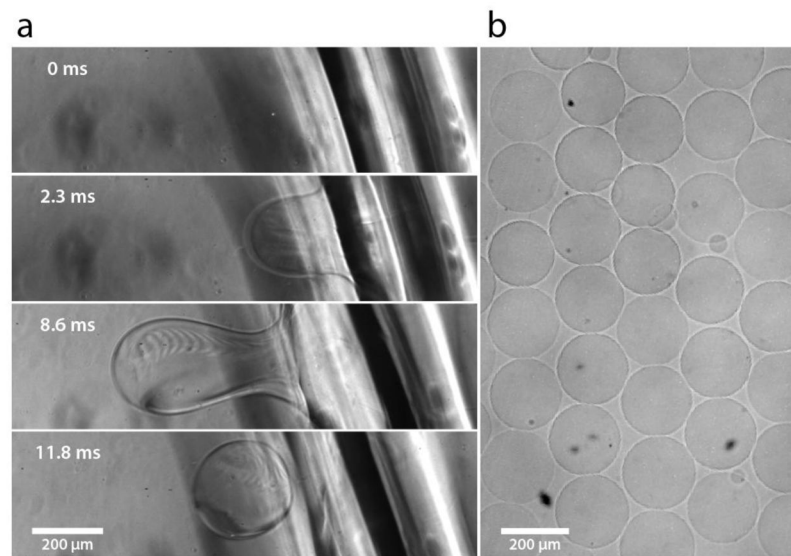


Figure 3. Vesicle Generation. Images of the vesicle generation process and several vesicles produced. (a) Deformation of the droplet interface bilayer (DPhPC) produced by rapid pulses of solution cause the membrane to pinch off and form a GUV. (b) Many vesicles generated using microfluidic jetting.