



HHS Public Access

Author manuscript

Contraception. Author manuscript; available in PMC 2015 August 24.

Published in final edited form as:

Contraception. 2013 September ; 88(3): 382–386. doi:10.1016/j.contraception.2012.10.034.

Effect of topical vaginal products on the detection of prostate-specific antigen, a biomarker of semen exposure, using ABACards^{☆,☆☆}

Margaret C. Snead^{a,*}, Athena P. Kourtis^a, Carolyn M. Black^a, Christine K. Mauck^b, Teresa M. Brown^a, Ana Penman-Aguilar^a, Johan H. Melendez^c, Maria F. Gallo^a, Denise J. Jamieson^a, and Maurizio Macaluso^d

^aDivision of Reproductive Health, National Center for Chronic Disease Prevention and Health Promotion, and the Division of Scientific Resources, National Center for Emerging and Zoonotic Infectious Diseases, Centers for Disease Control and Prevention, Atlanta, GA 30341, USA

^bCONRAD, Eastern Virginia Medical School (EVMS), Arlington, VA 23501, USA

^cJohns Hopkins University, Department of Infectious Diseases, Baltimore, MD 21224, USA

^dDivision of Biostatistics and Epidemiology, Cincinnati Children's Hospital Medical Center, Cincinnati, OH 45229, USA

Abstract

Background—Prostate-specific antigen (PSA) is a biomarker of recent semen exposure. There is currently only limited information on whether topical vaginal products affect PSA assays. We investigated this question using various dilutions of several vaginal products (lubricants and spermicides) and the Abacus ABACard for PSA detection.

Study Design—Pooled semen controls and various dilutions of nonoxynol-9 (N9), carboxymethyl cellulose (CMC), Replens, Gynol 2, K-Y jelly, Astroglide, Surgilube, combined with pooled semen dilutions, were tested for PSA using the Abacus ABACard.

Results—N9 (2% with saline) and CMC did not appear to affect the results of testing with the ABACard, but not all semen dilutions were tested. The other products (including Replens and Gynol, which is 2% N9 with propylene glycol, K-Y, Astroglide and Surgilube) at some of the dilutions tested either affected or gave invalid results with PSA testing using the ABACard. Both Gynol 2 and K-Y at 1:10 dilution gave false-positive results.

Conclusions—Some vaginal products affect PSA results obtained by using the semiquantitative ABACard. In vivo confirmation is necessary to further optimize PSA detection when topical vaginal products are present.

[☆]The findings and conclusions in this article are those of the authors and do not necessarily represent the official position of the Centers for Disease Control and Prevention.

^{☆☆}Use of trade names is for identification only and does not imply endorsement by the US Department of Health and Human Services.

^{*}Corresponding author. Centers for Disease Control and Prevention, Atlanta, GA 30341. Tel.: +1 770 488 6303; fax: +1 770 488 6391., msnead@cdc.gov (M.C. Snead).

Keywords

Vaginal products; PSA; Semen; Biomarker; ABACard; Lubricants; Spermicide

1. Introduction

Prostate-specific antigen (PSA) is a biomarker used to indicate recent vaginal semen exposure [1,2]. It is a sensitive and specific method for semen detection in women, originally developed for forensic purposes [3] and more recently adapted and utilized in reproductive health studies as an indicator of recent exposure to semen from unprotected sex or incorrect condom use [1,4–6]. PSA can be used as a marker to assess self-reported condom use as well as condom effectiveness [4] and, in clinical trials of contraception or sexually transmitted infections (STIs) and HIV prevention, as an indicator of adherence to study procedures (such as avoiding recent unprotected sex).

It is important to know whether spermicides or other vaginal products can affect the detection of PSA. In a clinical study of a new contraceptive diaphragm in which PSA was measured using the Abbott AXSYM® Microparticle Enzyme Immunoassay (Abbott Laboratories, Abbott Park, IL, USA), it appeared that nonoxynol-9 (N9) may have interfered with PSA detection [5]. There are other methods available for PSA detection. One is the Abacus OneStep ABACard (Abacus Diagnostics, West Hills, CA, USA) [6–8]. The card yields rapid and straightforward qualitative or semiquantitative results [9] and is relatively inexpensive.

Abacus OneStep ABACard is an antigen-specific monoclonal antibody membrane assay that has a lower limit of PSA detection of 4-ng PSA/mL vaginal swab eluent [7]. Although the card was originally developed as a qualitative assay, it has been used semiquantitatively [9] (Fig. 1), and its semiquantitative results correlated well with results of the quantitative Abbott IMX assay [9]. There is only limited evidence on the effect of vaginal products on PSA testing using ABACards. Given the lack of available information on this topic, as well as the important role that biomarkers of semen exposure can play in microbicide, HIV/STI prevention and contraception research, we undertook laboratory investigations to determine whether specific vaginal products affect PSA detection by ABACards.

2. Methods

2.1. In vitro experiments

Table 1 describes the vaginal products (lubricants and spermicides) that were tested: N9 (formulated at Eastern Virginia Medical School laboratory as 2% N9 in saline), carboxymethyl cellulose (CMC), Replens, Gynol (2% N9 with propylene glycol), K-Y, Astroglide and Surgilube.

First, positive controls (semen alone) were prepared by serially diluting [with phosphate buffer saline (PBS)] pooled semen stock, which had been stored at -80°C at a 1:50 dilution and then thawed. PBS was used as the diluting medium rather than what is supplied by the manufacturer as it is a commonly used diluting medium. Twofold dilutions were created and

tested (without vaginal products) by the ABACard starting with 1:1600 through 1:1,638,400. Semen alone was also tested with the Abbott Architect chemiluminescent quantitative immunoassay [10], in order to quantify the PSA concentration range for each dilution and correlate with the semiquantitative results obtained from ABACard.

Next, each of the vaginal products was mixed with semen. Each was diluted in PBS at 1:10 and 1:40 dilutions (Surgilube was also diluted at 1:20) and then added to the series of semen dilutions in equal volumes so that the final semen dilutions were twofold, ranging from 1:1600 through 1:1,638,400. For each of the samples tested with the ABACard, 200 μ L of an extract was placed in the test device, and all test results read at 10 min. Results were considered invalid if there was no control line visible within 10 min.

Last, negative controls, that is, products that had been mixed with PBS only (no semen and, therefore, expected to give negative PSA results) were also tested with the ABACards. All controls were tested on the same day as the products.

3. Results

The effects of the vaginal products on PSA detection by ABACard are presented in Table 2. N9 and CMC, at the semen dilutions tested, did not appear to affect PSA detection. Replens at the 1:10 dilution may have interfered slightly, with a weakly positive PSA result at the 1:102,400 semen dilution instead of the positive result that would have been expected based on the results of the semen-alone “positive control” and a negative result at the 1:204,800 dilution instead of the expected weakly positive one. However, at the 1:40 dilution, no effect was seen. Both Gynol and K-Y at 1:10 dilution had positive results at all semen dilutions, as well as false-positive results in the absence of semen; at the 1:40, dilution there was no effect of the products on PSA detection. All dilutions of Astroglide yielded invalid results. Surgilube produced invalid results at the 1:10 dilution but not at the 1:20 and 1:40 dilutions, which showed higher than expected results at the 1:204,800 semen dilution.

4. Discussion

The lower-than-expected results seen with Replens at a 1:10 dilution, if seen in a clinical trial, would give a woman with a vaginal concentration of PSA that was really 5.6–7.6 ng/mL, an apparent concentration of 3.0–3.9, and a woman with an actual concentration of 3.0–3.9 ng/mL, an apparent concentration of 2.0 ng/mL or less. The higher-than-expected results seen with Surgilube at 1:20 and 1:40 would mean that a woman with an actual concentration of 3.0–3.9 ng/mL would have an apparent concentration of 5.6–7.6 ng/mL. None of these differences would be likely to greatly affect interpretation of trial results if using quantitative PSA assays since cutoffs of 3 ng/mL or 1 ng/mL [11,12] are commonly used to indicate presence or absence of semen [1,13], particularly since the proportion of samples with low PSA has been small in previous studies [11,12], but is a concern when using the ABACards since their lower limit of detection is 4 ng/mL [7,9]. The false-positive results seen with Gynol and K-Y at 1:10 dilutions are of more concern, since a woman with no semen exposure at all would appear to have a concentration of 5.6–7.6 ng/mL.

Importantly, other than the lower-than-expected results seen with Replens at 1:10, there were no false-negatives or other indications that products inhibited detection of PSA. The invalid results produced by all dilutions of Astroglide and the 1:10 concentration of Surgilube were probably due to the viscosity of the products. These results were considered invalid because there was no control line visible within 10 min. It is unclear whether clinical specimens obtained from women who had used these products would give the same results as the in vitro experiments. Products in the experiment that either gave invalid results or false-positive results (such as K-Y, Gynol, Astroglide or Surgilube) especially need to be further evaluated when the ABACard is being used to assess PSA in vaginal fluids. If further evaluations confirm in vivo the effects of these products on ABACard results, then other PSA assays should be considered in populations where such product use is common.

The evidence on whether vaginal products or other substances affect PSA detection is limited and the results contradictory. Currently, the World Health Organization and general guidelines for forensic examinations recommend not using lubricants on specula during pelvic examination because they may affect forensic analysis [14]. Maher et al. [15] found an association between N9 and false-positive PSA results when using the biofilm membrane test. Sutton et al. [16] found that N9 and other substances (such as human milk, urine, feces and blood) potentially affected an Enzyme Linked Immunosorbent Assay (ELISA) for PSA detection, and using a similar assay, Johnson and Kobuwski [17] found false-negative results when samples were contaminated with common household detergents. In contrast, Stowell et al. [18] found no effect of menstrual blood, male or female saliva or female urine but did find that PSA recovery was affected by the presence of certain proteins found in body fluids using a sandwich ELISA. Melendez et al. [19] found that while some topical products (such as Silicorel, a silicone-based lubricant) did not affect the Abbott Architect's ability to detect PSA, other products (such as Replens and Gynol) seemed to inhibit detection (with lower-than-expected results), but the addition of K-Y jelly showed higher-than-expected results.

The literature on the effect of contaminants or other vaginal products on PSA detection using ABACard specifically is even more limited. Kristaly and Smith [20] did not find any effect when mixing blood and saliva with semen. Hochmeister et al. [7] similarly did not find an effect of various female body fluids, saliva or perspiration from male donors or anal swabs. Male urine was an exception, as expected, given the shared male genitourinary tract [7]. Pang and Cheung [21] did not find any effect of bodily fluids, lubricants or spermicides including N9 with PSA detection using the ABACard. On the other hand, Bitner [22] found that spermicidal lubricants affected the Seratec semiquantitative assay (membrane strip similar to ABACard assay) and recommended that this test not be used when testing the inside of a condom for PSA. Laffan et al. [23] evaluated body fluids and substrates (including lubricants) and found false-negative results only from caustic soda with the Seratec semiquantitative assay.

There are some limitations to our study. First, this was an in vitro experiment, and while we did our best to estimate the approximate amount of product that would potentially be present intravaginally (based on typical use and/or manufacturer's directions for use of the products), this remains an estimate. Not all of the vaginal products were tested for all of the

same semen dilution factors. PBS was used as the diluting medium rather than what is supplied by the manufacturer. Hobbs et al. [24] showed that using saline rather than that manufacturer's buffer did not affect results of the ABACard, although it did affect semenogelin detection using the Rapid Stain Identification Series for Semen Detection assay. In addition, how the results of a controlled laboratory experiment translate to real-life situations remain uncertain. Any diluting laboratory medium could be quite different from vaginal fluids in pH or other physicochemical characteristics. In vivo factors such as phase of the menstrual cycle, vaginal inflammation or infection or hormonal contraception may also affect some of the local parameters and lead to different results. The viscosity of particular products seems to have affected migration through the antigen-specific monoclonal antibody membrane used in the ABACard assay and, thus, affected the performance of the test. Our results are limited to PSA detection by ABACards; the effects of lubricants and other vaginal products on other PSA assays such as the quantitative Abbott assay warrants further study.

The importance of including biomarkers of semen exposure in sexual health studies has been argued by many investigators [2,13,25,26]. PSA is an excellent biomarker of recent (up to 48h) semen exposure [4,5] and could be very useful in future research as a marker of compliance with study procedures and as a way to assess self-reported condom use and condom failure.

In conclusion, Replens, Gynol, K-Y, Astroglide and Surgilube, at some of the dilutions tested, either affected or gave invalid results with PSA testing using the ABACard. Confirmation of the present results using actual clinical specimens will be an important next step. Future studies should consider the specific vaginal products used, such as lubricants, spermicides or microbicides, as well as the dose or amount of the product, when selecting an assay to detect PSA as a biomarker of recent semen exposure. Further considerations should also include the need to collect data on participants' product use when determining what (or if) PSA assays are to be used and the potential for misclassification. Similar considerations should apply to future use of PSA as a semen biomarker in the development of vaginal and rectal microbicides.

Acknowledgments

The authors would like to acknowledge Laurie Howard Jones and Edmund Gumisiriza for expert technical assistance as well as the CONRAD Clinical Working Group on Evaluation of Markers of Intercourse in Trials of Vaginal Barriers for helpful discussions.

No funding was received for this project or paper.

References

1. Mauck CK, Doncel GF. Biomarkers of semen in the vagina: applications in clinical trials of contraception and prevention of sexually transmitted pathogens including HIV. *Contraception*. 2007; 75:407–19. [PubMed: 17519146]
2. Gallo MF, Steiner MJ, Hobbs MM, Warner L, Jamieson DJ, Macaluso M. Biological markers of semen exposure: tools for improving the assessment of sexual behavior in HIV/STI prevention research. 2012 submitted to *AIDS & Behav*.

3. Graves H, Sensabaugh G, Blake E. Postcoital detection of a male-specific semen protein. Application to the investigation of rape. *N Engl J Med.* 1985; 312:338–43. [PubMed: 3881667]
4. Mauck CK, Weaver MA, Schwartz JL, Walsh T, Joanis C. Critical next steps for female condom research—report from a workshop. *Contraception.* 2009; 79:339–44. [PubMed: 19341844]
5. Rountree RW, Kilbourne-Brook M, Mauck CK, et al. SILCS diaphragm: postcoital testing of a new single-size contraceptive device. *Contraception.* 2008; 78:237–44. [PubMed: 18692615]
6. Culhane JF, Nyirjesy P, McCollum K, Casabellata G, Di Santolo M, Cauci S. Evaluation of semen detection in vaginal secretions: comparison of four methods. *Am J Reprod Immunol.* 2008; 60:274–81. [PubMed: 18647289]
7. Abacus Diagnostics, West Hills, CA. ABACard. [cited 2012 April 27]. Available from <http://www.abacusdiagnostics.com/semen.htm>
8. Hochmeister MN, Budowle B, Rudin O, et al. Evaluation of prostate-specific antigen (PSA) membrane test assays for the forensic identification of seminal fluid. *J Forensic Sci.* 1999; 44:1057–60. [PubMed: 10486959]
9. Hobbs MM, Steiner MJ, Rich KD, et al. Good performance of rapid prostate-specific antigen test for detection of semen exposure in women: implications for qualitative research. *Sex Transm Dis.* 2009; 36:501–6. [PubMed: 19455082]
10. Abbott Diagnostics, Abbott Park, IL. ARCHITECT i2000SR. [cited 2012 April 27]. Available from http://www.abbottdiagnostics.com/Products/Instruments_by_Platform/default.cfm?system=ARCHITECT&suffix=i2000sr®=us
11. Galvão LW, Oliveirac LC, Díaz J, et al. Effectiveness of female and male condoms in preventing exposure to semen during vaginal intercourse: a randomized trial. *Contraception.* 2005; 71:130–6. [PubMed: 15707563]
12. Macaluso M, Lawson LM, Hortin G, et al. Efficacy of the female condom as a barrier to semen during intercourse. *Am J Epidemiol.* 2003; 157:289–97. [PubMed: 12578798]
13. Macaluso M, Lawson L, Akers R, et al. Prostate-specific antigen in vaginal fluid as a biologic marker of condom failure. *Contraception.* 1999; 59:195–201. [PubMed: 10382083]
14. WHO Clinical management of rape survivors: developing protocols for use with refugees and internally displaced persons – Revised ed; Annex 7 Forensic Examination. p. 52 [cited 2012 April 27]. Available from http://www.searo.who.int/LinkFiles/Publications_clinical_mngt_rape_survivors.pdf
15. Maher J, Vintiner S, Elliot D, Melia L. Evaluation of the BioSign PSA membrane test for the identification of semen stains in forensic casework. *N Z Med J.* 2002; 115:48–9. [PubMed: 11942515]
16. Sutton JG, Bosley C, Rands A. The detection by Enzyme Linked Immunosorbent Assay of P30 and 19-OH Prostaglandin F1/F2, in the presence of a range of possible contaminants. *Sci Justice.* 1998; 38:157–64. [PubMed: 9800431]
17. Jothnson ED, Kotowski TM. Detection of prostate specific antigen by ELISA. *J Forensic Sci.* 1993; 38:250–8. [PubMed: 7681096]
18. Stowell LI, Sharman LE, Hamel K. An enzyme-linked immunosorbent assay (ELISA) for prostate-specific antigen. *Forensic Sci Int.* 1991; 50:125–38. [PubMed: 1718830]
19. Melendez, JH.; Doncel, GF.; Chaney, D.; Schwartz, JL.; Snead, MC.; Mauck, CK., et al. Inhibitory effect of lubricants and a vaginal contraceptive gel on detection of biomarkers of semen exposure. London: International Society for STD Research; 2009. abstract
20. Kristaly, A.; Smith, D. Report from Miami Dade Police Department. 1998. Validation of the One Step ABACard™ PSA test for the rapid forensic identification of semen.
21. Pang BC, Cheung BK. Identification of human semenogelin in membrane strip test as an alternative method for the detection of semen. *Forensic Sci Int.* 2007; 169:27–31. [PubMed: 16949235]
22. Bitner SE. False positives observed on the Seratec® PSA semiquant cassette test with condom lubricants. *J Forensic Sci.* 2012 Epub ahead of print.
23. Laffan A, Sawyer I, Quinones I, Daniel B. Evaluation of semen presumptive tests for use at crime scenes. *Med Sci Law.* 2011; 51:11–7. [PubMed: 21595415]

24. Hobbs MM, Steiner MJ, Rich KD, Gallo MF, Warner L, Macaluso M. Vaginal swab specimen processing methods influence performance of rapid semen detection tests: a cautionary tale. *Contraception*. 2010; 82:291–5. Epub 2010 Apr 13. [PubMed: 20705160]
25. Gallo MF, Steiner MJ, Hobbs MM, et al. Predictors of unprotected sex among female sex workers in Madagascar: comparing semen bio-markers and self-reported data. *AIDS Behav*. 2010; 14:1279–86. [PubMed: 20625928]
26. Minnis AM, Steiner MJ, Gallo MF, Warner L, Hobbs MM, van der Straten A, et al. Biomarker validation of reports of recent sexual activity: results of a randomized controlled study in Zimbabwe. *Am J Epidemiol*. 2009; 170:918–24. [PubMed: 19741042]

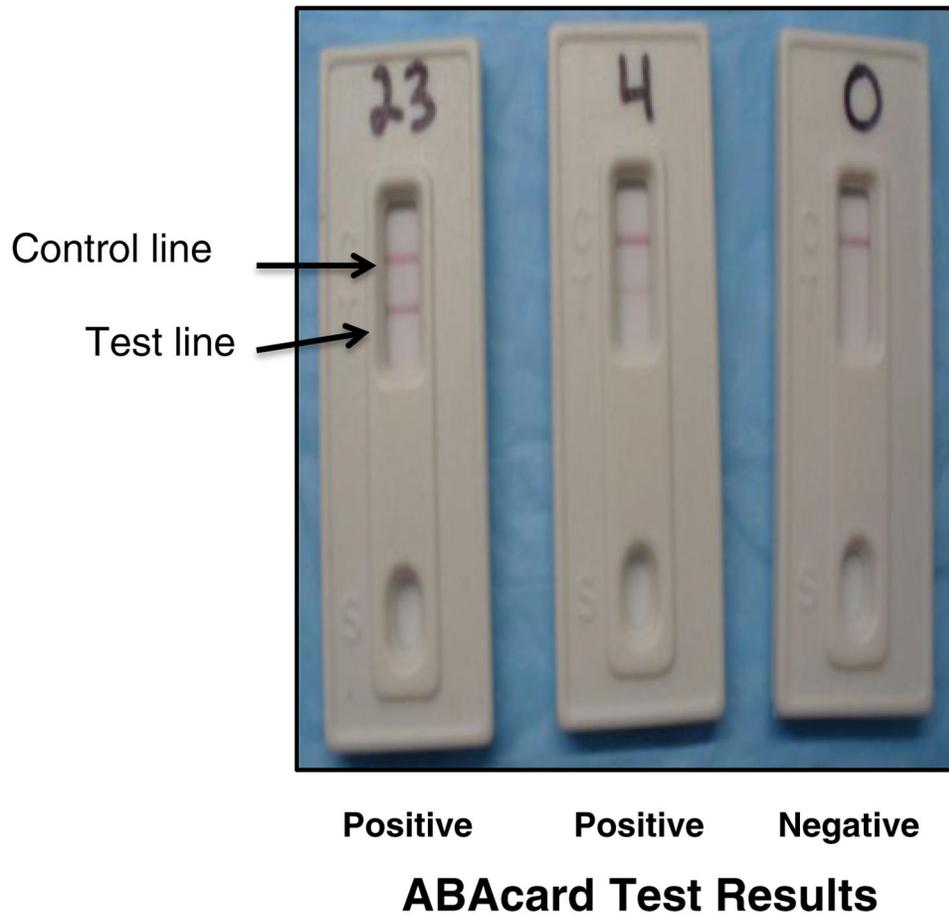


Fig. 1.
ABACard.

Table 1

Vaginal products included in the experiments of PSA detection by ABACards

| Product | Brand name (manufacturer) | Main ingredient | Type | Date tested |
|----------------|-------------------------------------|---|--------------------------------|--------------------|
| N9 | N/A (formulated @ EVMS) | N9 2% in saline | Spermicide | June 2009 |
| CMC | N/A (formulated @ EVMS) | CMC | Main ingredient for lubricants | June 2009 |
| Replens | Replens (LDS Consumer Products) | Polycarbofil | Vaginal lubricant | September 2009 |
| K-Y | K-Y Brand Jelly (Johnson & Johnson) | CMC | Vaginal lubricant | September 2009 |
| Astro | Astroglide (BioFilm, Inc) | Glycerin and propylene glycol | Vaginal lubricant | September 2009 |
| Gynol | Gynol 2 (Ortho) | N9 2% in propylene glycol | Spermicide | September 2009 |
| Surgi | Surgilube (Fougera) | Chlorexidine gluconate and natural water soluble gums | Surgical sterile lubricant | March 2010 |

N/A: not applicable; EVMS: Eastern Virginia Medical School.

Author Manuscript

Author Manuscript

Author Manuscript

Author Manuscript

Table 2

In vitro effect of vaginal products on PSA detection by ABACard

| Semen alone | Semen dilutions* | | | | | Product and amount |
|--------------|------------------|-----------|------------|------------|------------|------------------------|
| | 1: 3200 | 1: 51,200 | 1: 102,400 | 1: 204,800 | 1: 409,600 | |
| | + | + | + | +/- | - | No semen, product only |
| N9 1:10 | + | + | Nt | Nt | - | - |
| N9 1:40 | + | + | Nt | Nt | - | - |
| CMC 1:10 | + | + | Nt | Nt | - | - |
| CMC 1:40 | + | + | Nt | Nt | - | - |
| Replens 1:10 | + | + | +/- | - | - | - |
| Replens 1:40 | + | + | +/- | - | - | - |
| K-Y 1:10 | + | + | + | + | + | + |
| K-Y 1:40 | + | + | +/- | - | - | - |
| Astro 1:10 | Invalid | Invalid | Invalid | Invalid | Invalid | Invalid |
| Astro 1:40 | Invalid | Invalid | Invalid | Invalid | Invalid | Invalid |
| Gynol 1:10 | + | + | + | + | + | + |
| Gynol 1:40 | + | + | +/- | - | - | - |
| Surgi 1:10 | Invalid | Invalid | Invalid | Invalid | Invalid | Invalid |
| Surgi 1:20 | + | + | + | - | - | - |
| Surgi 1:40 | + | + | + | - | - | - |

+: positive, +/-: weakly positive, -: negative, Nt: not tested, N/A: not applicable.

* Semen alone was also tested with Abbott Architect quantitative assay. The PSA concentration (ng/mL) ranges for the semen dilutions as follows: 1: 3200=90.8->100-ng/mL, PSA vaginal swab eluent; 1: 51,200=1.6-14.8 ng/mL; 1: 102,400=5.6-7.6; 1: 204,800=3.0-3.9 (corresponds to the ABACard +/-due to 4 ng/mL lower level of detection); 1: 409,600=1.4-2.0; 1: 819,200=0.74-1.