



HHS Public Access

Author manuscript

J Occup Environ Hyg. Author manuscript; available in PMC 2018 May 01.

Published in final edited form as:

J Occup Environ Hyg. 2017 May ; 14(5): 368–376. doi:10.1080/15459624.2016.1263391.

Nonwoven Textile for Use in a Nanoparticle Respiratory Deposition Sampler

Donna J.H. Vosburgh^{1,*}, Jae Hong Park², Levi W. D. Mines², Imali A. Mudunkotuwa³, T. Renée Anthony², and Thomas M. Peters²

¹Department of Occupational and Environmental Safety and Health, University of Wisconsin-Whitewater, Whitewater, Wisconsin, USA

²Department of Occupational and Environmental Health, The University of Iowa, Iowa City, Iowa, USA

³Department of Chemistry, The University of Iowa, Iowa City, Iowa, USA

Abstract

The nanoparticle respiratory deposition (NRD) sampler is a personal sampler that combines a cyclone, impactor, and a nylon mesh diffusion stage to measure a worker's exposure to nanoparticles. The concentration of titanium in the nylon mesh of the diffusion stage complicates the application of the NRD sampler for assessing exposures to titanium dioxide nanoparticles. This study evaluated commercially available nonwoven textiles for use as an alternative media in the diffusion stage of the NRD sampler. Three textiles were selected as containing little titanium from an initial screening of 11 textiles by field portable x-ray fluorescence (FPXRF). Further evaluation on these three textiles was conducted to determine the concentration of titanium and other metals by inductively coupled plasma – optical emission spectroscopy (ICP-OES), the number of layers required to achieve desired collection characteristics for use as the diffusion stage in the NRD sampler (i.e., the nanoparticulate matter, NPM, criterion), and the pressure drop associated with that number of layers.

Only three (two composed of cotton fibers, C1 and C2; and one of viscose bamboo and cotton fibers, BC) of 11 textiles screened had titanium concentrations below the limit of detection the XRF device ($0.15 \mu\text{g}/\text{cm}^2$). Multiple metals, including small amounts of titanium, were found in each of the three nonwoven textiles using ICP-OES. The number of 25-mm-diameter layers required to achieve the collection efficiency by size required for the NRD sampler was three for C1 ($R^2 = 0.95$ with reference to the NPM criterion), two for C2 ($R^2 = 0.79$), and three for BC ($R^2 = 0.87$). All measured pressure drops were less than the theoretical and even the greatest pressure drop of 65.4 Pa indicated that a typical personal sampling pump could accommodate any of the three nonwoven textiles in the NRD sampler. The titanium concentration, collection efficiency, and measured pressure drops show there is a potential for nonwoven textiles to be used as the diffusion stage of the NRD sampler.

*Corresponding author: Donna J.H. Vosburgh.

Keywords

nanoparticle; nonwoven; textile; sampler; diffusion

INTRODUCTION

Airborne nanoparticles—particles with a diameter of at least one dimension smaller than 100 nm⁽¹⁾—are present in many workplaces. Measuring nanoparticle exposure in the workplace is challenging and has involved multiple types of instruments and sampling strategies.⁽²⁾ Ideally what is needed is a sampler that fits into current industrial hygiene field sampling methodologies, particularly one that is small enough to be used to assess personal exposures⁽³⁾, can allow quantification of nanoparticles apart from larger particles that occur in the work environment, and collects nanoparticles with an efficiency that matches respiratory deposition.⁽⁴⁾

The nanoparticle respiratory deposition (NRD) sampler is a new personal sampler that was developed to streamline nanoparticle exposure assessment.⁽⁴⁾ The NRD sampler is composed of three parts: a 25-mm aluminum respirable cyclone, an impaction stage, and a diffusion stage. The diffusion stage consists of eight nylon mesh screens with a collection efficiency by particle size closely matching the nano-particulate matter (NPM) criterion deposition of nanoparticles smaller than 300 nm. The NPM criterion was developed by Cena et al.⁽⁴⁾ from the International Commission on Radiological Protection deposition curve for the average adult under light exercise and nose-breathing conditions⁽⁵⁾ and represents the fraction of NPM that can deposit in the respiratory system when inhaled.⁽⁴⁾ The NRD sampler is commercially available (ZNRD001, Zefon, UAS) and work has been done to establish a method for using the NRD sampler to evaluating exposure to welding fumes.⁽⁶⁾

Although the NRD sampler works well to collect nanoparticles with an efficiency that matches the respiratory system, the nylon mesh screen in the diffusion stage contain high levels of titanium, presumably as titanium dioxide (TiO₂), used to whiten the nylon.⁽⁷⁾ Measuring occupational exposure to nano-sized TiO₂ aerosol is of interest for many industrial hygienists because nano-sized TiO₂ is used in many commercial products, commonly as a whitener, and has been classified as a potential occupational carcinogen.⁽⁸⁾ The mass of collected TiO₂ that can be differentiated from the background metal in the collection media, the limit of detection (LOD) of the media, is an important consideration. For a sample collected over eight hours with the 2.5 L min⁻¹ NRD sampler, the diffusion media must contain less than 14.8 µg total titanium to quantify airborne nano-sized TiO₂ at one-tenth of the National Institute for Occupational Safety and Health (NIOSH) recommended exposure limit (REL) of 0.3 mg m⁻³. The commercial NRD sampler is not able to be used to measure those occupational exposures because of the large amounts of titanium on the diffusion stage.⁽⁷⁾

Nonwoven textiles are a potential media for in the diffusion stage of the NRD sampler. A nonwoven textile is a fabric composed of fibers that are randomly oriented and held together by means other than weaving or knitting.⁽⁹⁾ Nonwoven textiles can be composed of a variety of materials including natural fibers, such as cotton, and manmade fibers, such as polyester.

The collection efficiency of nonwoven textiles depends on the textile characteristics of basis weight, fiber diameter, material thickness, and material fiber density.⁽¹⁰⁾ Basis weight is a textile term that refers to the mass of a surface area of fabric.⁽¹¹⁾ The packing density of nonwoven textiles varies and may be low enough to allow for the diffusion stage to match the NPM criterion while remaining small enough to fit in the NRD sampler.

In this study, we investigated the use of nonwoven textiles in the diffusion stage of the NRD sampler. For the nonwoven textiles to be useful in the NRD sampler, they would have to have either no or a very low concentration of titanium, an aerosol collection efficiency that matched the NPM criterion, and a pressure drop small enough that a personal pump could be used. We first screened a variety of commercially available textiles for titanium using field portable X-ray fluorescence (FPXRF). On selected nonwoven textiles below the LOD of the FPXRF, additional testing was conducted. The physical characteristics of the nonwoven textiles (basis weight, fiber diameter, textile thickness, and material density) were determined and used to theoretically estimate the quantity of each nonwoven textile needed to achieve the required particle collection efficiency in the 2.5 L min⁻¹ NRD sampler along with the pressure drop caused by that amount of nonwoven textile. The metals content was measured by traditional digestion and metals analysis methods. Then the measured collection efficiency and pressure drop for the selected nonwoven textiles was determined in laboratory experiments.

METHODS

As presented in Table I, eleven nonwoven textiles (i.e., quilt battings) were selected as inexpensive, readily-available nonwoven textiles with the potential to replace the nylon mesh in the diffusion stage of the NRD sampler. Manufactured by two companies (Quilters Dream Batting, Virginia Beach, VA; and Pellon Consumer Products, Clearwater, FL), these nonwoven textiles represent a cross-section of available batting colors (five white, one black, and five off-white) and composition (four polyester, two wool, two cotton, two mixed, one fire-retardant fibers). These nonwoven textiles were produced by needle-punching, a process to mechanical interlock the fibers and hold them together without adhesive.

A FPXRF (Niton XL3t Ultra, Thermo Scientific, Waltham, MA, USA) was used to screen nonwoven textiles for titanium. Nonwoven textiles with titanium compositions greater than LOD of the FPXRF were removed from further testing. The limit of detection of titanium for the FPXRF is 0.15 µg/cm². The FPXRF was set to thin film standard filter mode with a sample duration of 120 seconds (main range: 40 seconds, low range: 40 seconds, and high range: 40 seconds). Three measurements (upper left corner, middle, lower right corner) were taken on one piece (5.1 cm × 5.1 cm) of each of the 11 nonwoven textiles.

Physical Characterization

The nonwoven textiles selected for further evaluation were characterized physically to determine the textile thickness, basis weight, fiber material density, and fiber diameter of each nonwoven textile so that the collection efficiency of particles smaller than 300 nm and pressure drop could be estimated from filtration theory. The uncompressed thickness of each textile was measured with a caliper. The basis weight of ten squares (5.1 cm × 5.1 cm) of the

nonwoven textile was calculated as the weight divided by the surface area of the square (25.8 cm²). Fiber material densities were obtained from literature.^(12,13) For nonwoven textiles containing fibers of mixed fiber composition, the fiber material density was calculated based on the percentages of fibers listed by the manufacturer.

The diameter of individual fibers in each nonwoven textile was determined using scanning electron microscopy (SEM) (S4800, Hitachi-High Technologies Corporation, Japan). Each nonwoven textile (1 cm × 1 cm) was placed on a stub and introduced inside a Sputter Coater (K550X, Quorum Technologies Ltd, UK) where a thin layer of Au/Pd (80%/20%) was deposited on to the nonwoven textile surface. This step was conducted in order to prevent excessive charging of the nonwoven textile during the analysis. Once the coating is complete, the nonwoven textile was imaged with 5.0 kV accelerating voltage and ImageJ (US National Institutes of Health, US) was used in image processing.

Theoretical Collection Efficiency

Filtration theory was used to determine the number of layers of each nonwoven textile required in the commercial NRD sampler (which is designed for a flow of 2.5 L min⁻¹ and a cassette diameter of 25 mm) for the sampler to achieve the NPM criterion. First the collection efficiency by particle diameter for one layer of each nonwoven textile was determined using the physical characteristics of each nonwoven textile. Then additional layers of nonwoven textile were added into the theory until the theoretical collection efficiency by particle size was close to the NPM criterion. The physical characteristics of the nonwoven textiles were applied to filtration theory when the solid volume fraction was estimated for nonwovens using Payen et al.⁽¹⁰⁾:

$$\alpha = 100 \frac{G}{L\rho_f} \quad [1]$$

where G is the basis weight of the nonwoven textile, L is the nonwoven textile thickness, and ρ_f is the fiber material density.

Following Raynor et al.⁽¹⁴⁾ the theoretical collection efficiency by particle diameter (E_T) of the three selected nonwoven textiles was computed as:

$$E_T = 1 - \exp\left(\frac{-4E_F\alpha L}{\pi d_f}\right) \quad [2]$$

where E_F is the single fiber efficiency, α is the solid volume fraction calculated using equation 1, and d_f is the fiber diameter. E_F was calculated as:

$$E_F = E_D + E_R \quad [3]$$

where E_D is the single fiber efficiency due to diffusion and E_R is the single fiber efficiency due to interception. The effects of inertial impaction and gravitational settling were neglected because particles of interest were smaller than 300 nm. The single fiber efficiency E_D was calculated as:

$$E_D = 1.6 \left(\frac{1 - \alpha}{Ku} \right) Pe^{-\frac{2}{3}} C_{C(d)} \quad [4]$$

where Pe is the Peclet number⁽¹⁴⁾, Ku is the Kuwabara hydrodynamic factor⁽¹⁴⁾, and $C_{C(d)}$ is the Cunningham slip correction factor calculated as:

$$C_{C(d)} = 1 + 0.388 Kn_f \left(\frac{(1 - \alpha) Pe}{Ku} \right)^{\frac{1}{3}} \quad [5]$$

In Equation 5, Kn_f is the Knutsen number of the nonwoven textile fiber. E_R was calculated as:

$$E_R = \left(\frac{1+R}{2Ku} \right) \left[2 \ln(1+R) - 1 + \alpha + \left(\frac{1}{1+R} \right)^2 \left(1 - \frac{\alpha}{2} \right) - \left(\frac{\alpha}{2} \right) (1 - R)^2 \right] \quad [6]$$

where R is the ratio of the particle diameter to the particle fiber. A flow rate of 2.5 L min⁻¹ was used to match that of the NRD sampler.⁽³⁾

Because the diffusion stage is downstream of the impactor in the NRD, the theoretical collection efficiency from above was adjusted ($E_{t,adj(d)}$) to account for collection that occurs in the impaction stage as:

$$E_{t,adj(d)} = E_{t(d)} P_{imp(d)} \quad [7]$$

where $P_{imp(da)}$ is the penetration through the impaction stage. $P_{imp(da)}$ was calculated as⁽¹⁵⁾:

$$P_{imp(da)} = 1 + \frac{\ln(da 10^6)}{8.65} + 0.15, d_a \leq 133.3 \text{ nm} \quad [8]$$

$$P_{imp(da)} = 1 - 0.46 \left(1 + \operatorname{erf} \left(\frac{\ln \left(\frac{d_a 10^6}{0.45} \right)}{\sqrt{2} \ln(1.43)} \right) \right) - 0.08, d_a > 133.3 \text{ nm} \quad [9]$$

where d_a is the aerodynamic diameter in meters. The d_a was converted to the mobility diameter, d , using Equations 10 and 11⁽¹⁶⁾:

$$d_v = d_a \sqrt{\frac{\chi \rho_0 C_c(d_a)}{\rho_p C_c(d_v)}} \quad [10]$$

$$d = d_v \frac{\chi C_c(d)}{C_c(d_v)} \quad [11]$$

where d_v is the volumetric diameter, χ is the dynamic shape factor (χ was assumed to be 1.08 for salt particles⁽¹⁶⁾), ρ_0 was the unit density (1000 kg m^{-3}) and ρ_p was assumed to be 2200 kg m^{-3} for salt particles.⁽¹⁶⁾

Experimental Collection Efficiency

For each of the selected nonwoven textiles, the collection efficiency by particle size for the textile specific number of layers computed from theory, was measured using the set up shown in Figure 1. Discs with diameters of 25 mm were cut from sheets of the nonwoven textiles and fixed in a holder (25-mm conductive polypropylene cassette). A nebulizer (Aeroneb Solo, Aerogen, Dangan, Ireland) was used to aerosolize a solution of 0.1% NaCl. The test aerosol was neutralized with a Kr-85 aerosol neutralizer (3054A, TSI Incorporated, Shoreview, MN), dried with a diffusion dryer, and then delivered into a 200 L coagulation chamber to. A fast mobility particle sizer (FMPS) (Model 3091, TSI Incorporated, Shoreview, MN) was used to measure the particle number concentration by mobility size using a 3-way valve to alternate without (WO) or with (W) the layer or layers of nonwoven textile being tested inline before the FMPS in the following sequence: $WO_1, W_1, WO_2, W_2, WO_3, W_3, WO_4$. The sampling airflow rate of the FMPS was 10 L min^{-1} , comprised of the 2.5 L min^{-1} through the nonwoven textile plus 7.5 L min^{-1} of clean HEPA-filtered air. The collection efficiency ($E_{exp(d)}$) of each nonwoven textile was calculated by using equation 12.

$$E_{exp(d)} = 1 - \left[\frac{W_1}{(WO_1 + WO_2)/2} + \frac{W_2}{(WO_2 + WO_3)/2} + \frac{W_3}{(WO_3 + WO_4)/2} \right] / 3 \quad [12]$$

The measured collection efficiency was then adjusted ($E_{exp,adj(d)}$) to account for collection that occurred in the impaction stage of the NRD using equation 13

$$E_{exp,adj(d)} = E_{exp(d)} P_{imp(d)} \quad [13]$$

Data Analysis

The adjusted measured collection efficiency was compared to the NPM criterion and the adjusted measured collection efficiency was also compared to the adjusted theoretical collection efficiency by calculating R^2 values. The R^2 of the $E_{exp,adj(d)}$ and the NPM curve

was calculated using equation 14 where $E_{exp,adj(d),avg}$ is the mean of the adjusted measured collection efficiency.

$$R_{exp,adj(d)-NPM}^2 = 1 - \frac{\sum (E_{exp,adj(d)} - NPM_{(d)})^2}{\sum (E_{exp,adj(d)} - E_{exp,adj(d),avg})^2} \quad [14]$$

The R^2 of the $E_{exp,adj(d)}$ and $E_{th,adj(d)}$ was calculated using equation 15.

$$R_{exp,adj(d)-adj(d)}^2 = 1 - \frac{\sum (E_{exp,adj(d)} - E_{adj(d)})^2}{\sum (E_{exp,adj(d)} - E_{exp,adj(d),avg})^2} \quad [15]$$

Pressure Drop

The pressure drops across each of the nonwoven textiles, P , was calculated for a flow rate of 2.5 L min^{-1} as:

$$\Delta P = \frac{16\eta\alpha UL}{Ku d_f^2} \quad [16]$$

where μ_a is the viscosity of air and U is the airflow rate.⁽¹⁴⁾

For each of the three selected nonwoven textiles, the pressure drop across one layer was experimentally determined by connecting a digital manometer (Series 475 Mark III, Dwyer Instruments, Inc., Michigan City, IN) upstream and downstream of a 25-mm conductive cassette while air was pulled through the cassette at 2.5 L min^{-1} . All measurements were conducted in triplicate.

Traditional Chemical Characterization

Inductively coupled plasma with optical emission spectroscopy (ICP-OES; model 720 ES, Varian, Inc., US) was used to measure the levels of titanium, chromium, manganese, iron, copper, and zinc in each of the three selected nonwoven textiles. As described in detail by Mudunkotuwa et al.⁽¹⁷⁾, a sample of textile (~ 200 – 400 mg) was inserted into a digestion vessel containing concentrated H_2SO_4 (4 mL) and concentrated HNO_3 (2 mL). The vessel was then placed in a microwave digestion system (MARS 6, CEM Corporation, USA). The temperature was ramped to 210°C , held for 45 minutes, and allowed to cool to room temperature. The resulting clear solution was then topped to 25 mL with water and analyzed. All measurements were conducted in triplicate.

Once the number of layers of each of the selected nonwoven textiles were verified by experimental collection efficiency, the LOD of each of the nonwoven textiles and each

element were calculated. The LOD was calculated by calculating the value three standard deviations of metal in the blank above the mean ICP-OES determined metal value in the pristine nonwoven textiles.⁽⁶⁾

RESULTS

Of the eleven nonwoven textiles, only three nonwoven textiles had titanium concentrations below the LOD for the FPXRF (Table I). All of the nonwoven textiles that were white or black in color had titanium concentrations above the LOD of the FPXRF. The three nonwoven textiles that had titanium concentrations below the FPXRF LOD were composed of natural cotton fibers or cotton blended with viscose bamboo fibers.

The characteristics of thickness, mean basis weight, and fiber material density of the three selected nonwoven textiles are shown in Table II. Since the BC nonwoven textile was composed of 50% viscose bamboo and 50% cotton, the mean of cotton⁽¹²⁾ and viscose bamboo⁽¹³⁾ was used for the fiber material density of the BC nonwoven textile. The results of fiber diameter determined by SEM are shown in Figure 2. The mean diameters range from 10.8 μm to 12.1 μm . C1 and C2 are composed of only fibers that are not cylindrical, while BC has both cylindrical and twisted, crimped fibers. Long and twisted fibers with convolutions, or crimps, in the middle of the fiber are typical of cotton fibers.⁽¹¹⁾

The size distribution of the salt test aerosol used to determine the measured collection efficiency of the selected nonwoven textiles is shown in Figure 3. The distribution of the test particles was lognormally distributed. The number mean and mode diameters were near 100 nm. The concentration and sized distribution of the test particles were stable during the experiment.

Adjusted collection efficiencies measured experimentally and theoretically compared to the NPM criterion are provided in Figure 4. Each textile required a different number of layers to achieve the NPM criterion. Nonwoven textile C1 required three layers, C2 required two layers, and BC required three layers to achieve good alignment with the NPM criterion. The shape of the measured collection efficiency for the required number of layers matched well with the NPM criterion. The adjusted measured collection efficiencies of the nonwoven textiles had good alignment with the NPM criterion with R^2 values of 0.95 for C1, 0.79 for C2, and 0.88 for BC. The adjusted measured collection efficiencies of the nonwoven textiles to the theory had R^2 values of 0.93 for C1, 0.88 for C2, and 0.79 for BC.

The theoretical pressure drop for one layer of each nonwoven textile was 19.2 Pa for C1, 32.7 Pa for C2, and 17.6 Pa for BC. The measured pressure drops of each of the three nonwoven textiles were 15.8 Pa, 21.6 Pa, and 13.3 Pa respectively. All of the measured pressure drops were less than the theoretical pressure drops. The pressure drop for one layer of C2 was the greatest, which agrees with the nonwoven textile characteristics (Table II) in that C2 was the thickest and had the largest basis weight. The total pressure drop for a diffusion stage composed of three layers of C1 was estimated at 57.7 Pa, two layers of C2 at 65.4 Pa, and three layers of BC at 52.7 Pa.

The ICP-OES results showed titanium in the nonwoven textiles. The titanium amounts listed in Table II equate to the mean amounts per one 25 mm circle of each of the nonwoven textiles; 0.26 μg for C1, 1.93 μg for C2, and 0.72 μg of titanium for the BC. The calculated LOD of the three nonwoven textiles were as follows: 0.78 μg for three layers of C1, 6.5 μg for two layers of C2, and 2.8 μg for three layers of BC.

DISCUSSION

Nonwoven textiles have the potential to serve as the media in the diffusion stage of the NRD sampler. The calculated LOD of titanium for the three selected nonwoven textiles after screening was substantially less than the 14.8 μg target value. The adjusted measured collection efficiency for all three nonwoven textiles was relatively close to the NPM (Figure 4) with R^2 values close to 1. The pressure drop per diffusion stage for each nonwoven textile was sufficiently small that any of the three materials could be used in the NRD sampler with a personal pump.⁽⁴⁾

To ensure nonwoven textiles met the requirement for titanium composition (less than one tenth of the REL), the target amount in the diffusion stage of an NRD sampler required an amount less than 14.8 μg titanium background. Although the FPXRF did not detect any titanium in three nonwoven textiles, the ICP-OES detected titanium in these materials (Table II). The amounts of the other measured metals in the nonwoven textiles were, in some cases, considerable: except for chromium in C1, the metals concentrations in one nonwoven textile layer were greater than the estimated limit of detection for NIOSH method 7300,⁽¹⁸⁾ indicating significant background contamination potential. The metal content of the nonwoven textiles would limit their use in certain occupational areas such as assessing welding fume exposure, which has already been identified as a potential use of the NRD sampler.⁽⁶⁾

The adjusted collection efficiency and pressure drops measured experimentally for all selected textiles were compatible for use in the NRD sampler. However, a nonwoven textile specifically developed for the NRD sampler may be needed. If natural fibers are used, the fiber shape may influence the collection efficiency in a way that may be unpredictable. Natural fibers that are long enough to be used in a nonwoven textile will not be perfectly cylindrical, and in some cases, such as with cotton, may be twisted and have many convolutions.⁽¹¹⁾ Natural fibers that have been processed, such as viscose bamboo fibers, may provide better agreement due to the cylindrical structure of the fibers.⁽¹³⁾ An alternative is to use newer techniques to create cylindrical fibers, such as electrospinning.^(19,20) Future research is needed to determine the influence of the fiber shape on collection efficiencies for diffusion layers in the NRD.

Before a nonwoven textile could be used in the NRD sampler, there are limitations that must be addressed. First, commercially available nonwoven materials with other intended purposes, such as the nonwoven textiles used in this study, may have variability in the product that could affect the homogeneity of the material. That variability has the potential of influencing the collection efficiency of a material. More work is needed to address the issue of humidity and fiber diameter for potential nonwoven fabrics. Natural fibers and hairs

were previously evaluated as an aerosol collection substrate⁽²¹⁾, but these authors identified a change in fiber characteristics with humidity. Some manmade fibers are more stable in their diameters with regard to humidity changes than others. Viscose bamboo has been shown to be to swell when wet, thereby increasing the fiber diameter, which may reasonably affect collection efficiency. However it is unknown if the fibers would absorb enough moisture from humidity to significantly increase their diameters.⁽¹³⁾ Particles smaller than 25 nm were not used when evaluating collection efficiencies of the nonwoven textiles. A workplace may have a significant amount of nanoparticles with diameters \geq 25 nm so additional collection efficiency assessments are recommended in this size range.

CONCLUSION

This work demonstrates that some nonwoven textiles are sufficiently free of metals contamination and can be used to achieve required collection characteristics for use as the diffusion stage of the NRD sampler. Three of eleven commercially available nonwoven textiles were selected to potentially replace the nylon mesh in the diffusion stage of the NRD sampler based on low metals content determined by FPXRF. The selected textiles can be used to achieve adjusted collection efficiencies compatible with the NPM criterion and at pressure drops sufficiently small for use with personal, belt-mounted sampling pumps. Although titanium was not detected in the three nonwoven textiles by FPXRF, it was detected by with the more sensitive ICP-OES. The LOD for all three of the materials were below the target value of 14.8 μg . However considerable amounts of other metals were detected in all of the three materials. The metal content of these commercially available nonwoven textiles would limit their use in assessing exposures to many common metals.

Acknowledgments

This research was funded by support from the National Institute for Occupational Safety and Health (R01 OH010238).

References

1. ASTM Standard E2456. Standard Terminology Relating to Nanotechnology. ASTM International; West Conshohocken, PA: 2006. www.astm.org
2. Ramachandran G, Ostraat M, Evans DE, Methner MM, O'Shaughnessy P, D'Arcy JD, Geraci CL, Stevenson E, Maynard A, Rickabaugh K. A Strategy for Assessing Workplace Exposures to Nanomaterials. *Journal of Occupational and Environmental Hygiene*. 2011; 8:673–685. [PubMed: 22023547]
3. Department of Health and Human Services, National Institute for Occupational Safety and Health. NIOSH Manual of Analytical Methods, Second Supplement, Chapter E-Development and Evaluation of Methods. 1998. (DHHS (NIOSH) Publication No. 98-119) Retrieved from <http://www.cdc.gov/niosh/docs/2003-154/pdfs/chapter-e.pdf>
4. Cena LG, Anthony TR, Peters TM. A Personal Nanoparticle Respiratory Deposition (NRD) Sampler. *Environ Sci Technol*. 2011; 45:6483–6490. [PubMed: 21718022]
5. International Commission on Radiological Protection (ICRP). Human Respiratory Tract Model for Radiological Protection. Elsevier Science, Ltd.; Oxford, U.K: 1994. Publication 66
6. Cena LG, Keane MJ, Chisholm WP, Stone S, Harper M, Chen BT. A Novel Method for Assessing Respiratory Deposition of Welding Fume Nanoparticles. *Journal of Occupational and Environmental Hygiene*. 2014; 11:771–780. [PubMed: 24824154]

7. Mines LWD, Park JH, Mudunkotuwa IA, Anthony TR, Grassian VH, Peters TM. Porous Polyurethane Foam for Use as a Particle Collection Substrate in a Nanoparticle Respiratory Deposition Sampler. *Aerosol Science and Technology*. 2006; 50:497–506.
8. Department of Health and Human Services, National Institute for Occupational Safety and Health. Current Intelligence Bulletin 63 Occupational Exposure to Titanium Dioxide. 2011. (DHHS (NIOSH) Publication No. 2011-160) Retrieved from <http://www.cdc.gov/niosh/docs/2011-160/pdfs/2011-160.pdf>
9. INDA Association of the Nonwoven Fabrics Industry. INDA. Cary, NC: 2002. INDA Nonwoven Glossary.
10. Payen J, Vroman P, Lewandowski M, Perwuelz A, Calle-Chazelet S, Thomas D. Influence of fiber diameter, fiber combinations and solid volume fraction on air filtration properties in nonwovens. *Textile Research Journal*. 2012; 82:1948–1959.
11. Morton, WE., Hearle, JWS. Physical properties of textile fibres. 4th. Woodhead Publishing Limited; Cambridge: 2008.
12. Zupin, Z., Dimitrovski, K. Mechanical Properties of Fabrics from Cotton and Biodegradable Yarns Bamboo, SPF, PLA in Weft. In: Dubrovski, PD., editor. Woven Fabric Engineering. InTech; 2010. p. 25-46.
13. Lipp-Symonowicz B, Sztajnowski S, Wojciechowska D. New Commercial Fibres Called 'Bamboo Fibres' - Their Structure and Properties. *Fibres & Textiles in Eastern Europe*. 2011; 19:18–23.
14. Raynor, PC., Leith, D., Lee, KW., Mukund, R. Sampling and Analysis Using Filters. In: Kulkarni, P. Baron, P., Willeke, K., editors. *Aerosol Measurements*. 3rd. Hoboken, New Jersey: John Wiley & Sons, Inc.; 2011. p. 107-128.
15. Park JH, Mudunkotuwa IA, Mines LWD, Anthony TR, Grassian VH, Peters TM. A granular bed for use in a nanoparticle respiratory deposition sampler. *Aerosol Science and Technology*. 2015; 49:179–187. [PubMed: 26900208]
16. Hinds, WC. *Aerosol Technology*. 2nd. John Wiley and Sons, Inc.; New York: 1999.
17. Mudunkotuwa I, Anthony TR, Grassian V, Peters TM. Accurate Quantification of TiO₂ Nanoparticles Collected on Air Filters Using a Microwave-Assisted Acid Digestion Method. *Journal of Occupational and Environmental Hygiene*. 2015; :1–28. DOI: 10.1080/15459624.2015.1072278 [PubMed: 24918755]
18. Department of Health and Human Services, National Institute for Occupational Safety and Health. NIOSH Manual of Analytical Methods, Third Supplement. 2003. (DHHS (NIOSH) Publication No. 2003-154) Retrieved from <http://www.cdc.gov/niosh/docs/2003-154/>
19. Wang N, Raza A, Si Y, Yu J, Sun G, Ding B. Tortuously structured polyvinyl chloride/polyurethane fibrous membranes for high-efficiency fine particle filtration. *Journal of Colloid and Interface Science*. 2013; 398:240–246. [PubMed: 23489615]
20. Yun KM, Hogan CJ Jr, Matsubayashi Y, Kawabe M, Iskandar F, Okuyama K. Nanoparticle filtration by electrospun polymer fibers. *Chemical Engineering Science*. 2007; 62:4751–4759.
21. Jackson GW, James DF. The Permeability of fibrous porous media. *The Canadian Journal of Chemical Engineering*. 1986; 64:364–374.

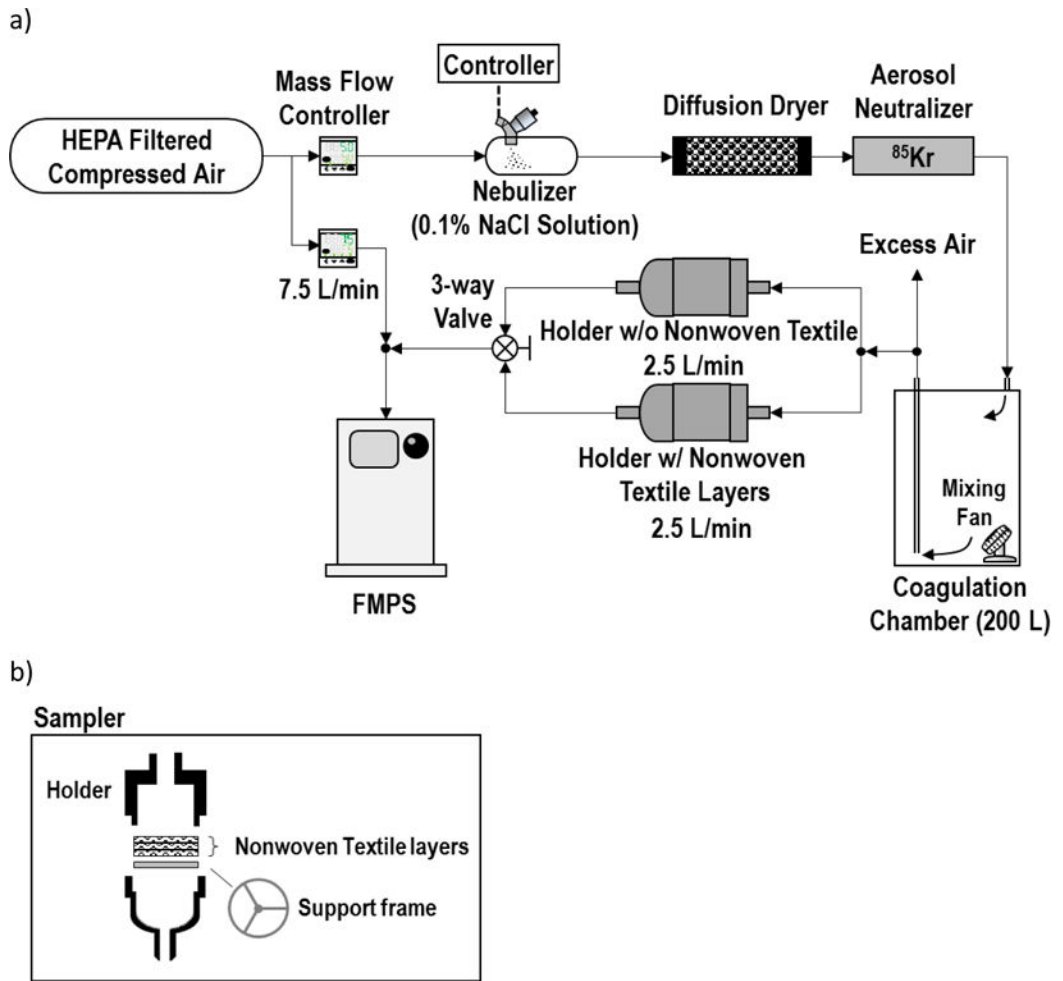
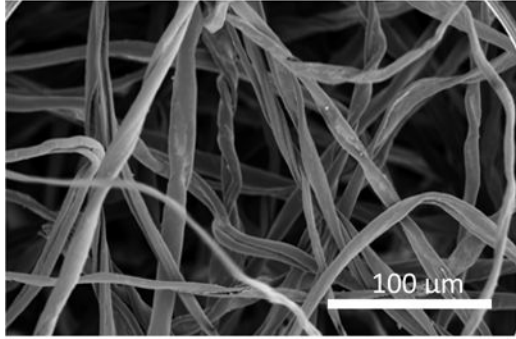
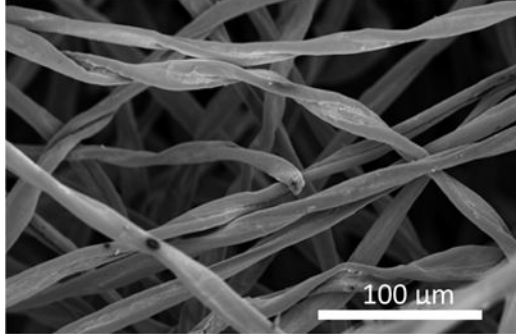
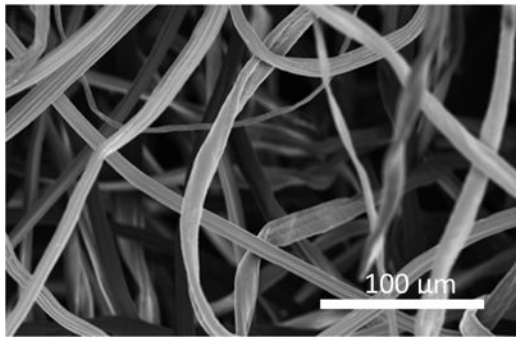


FIGURE 1. Evaluation of particle collection efficiency of nonwoven textiles: a) experimental set up b) diagram of sampler.

a) Nonwoven textile C1: 10.8 μm (5.7)b) Nonwoven textile C2: 11.4 μm (3.7)c) Nonwoven textile BC: 12.1 μm (3.3)**FIGURE 2.**

Scanning electron microscopy images, with the mean (standard deviation) of one fiber diameter, of the three nonwoven textiles: a) Quilters Dream Cotton, C1; b) Pellon Natural Cotton, C2; and c) Pellon Viscose Bamboo, BC.

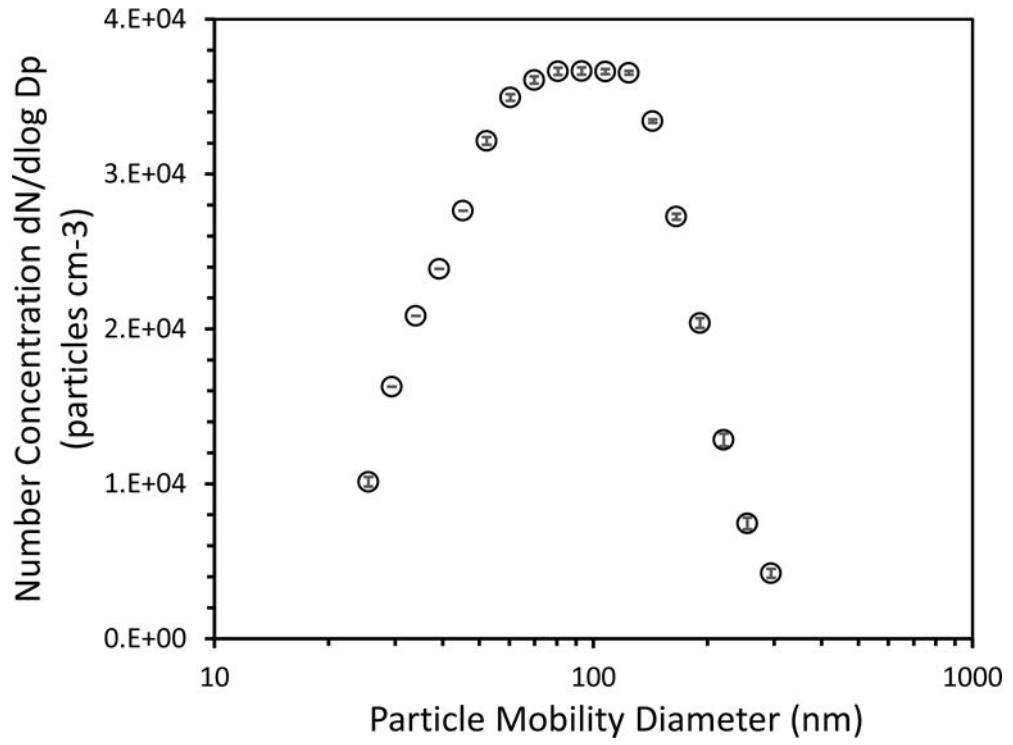


FIGURE 3. Particle number concentration by particle mobility diameter for salt aerosol used to test efficiency of nonwoven textiles. Error bars represent one standard deviation of twelve measurements.

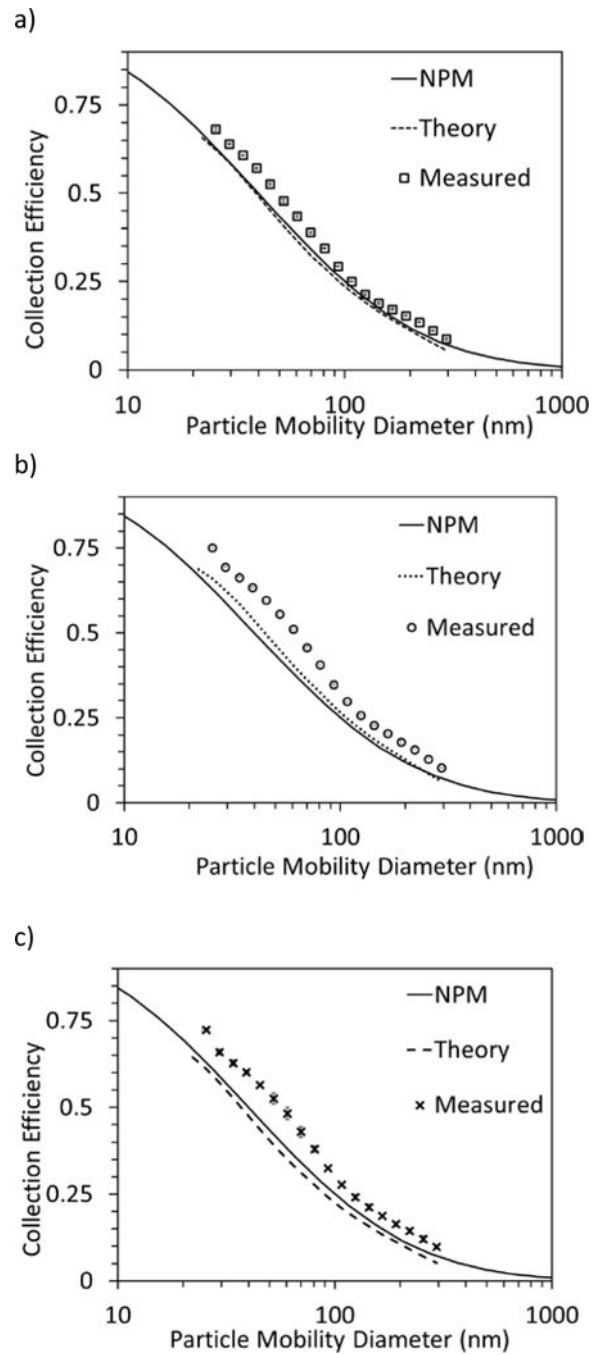


Figure 4. Impactor adjusted theoretical (dashed) and measured (symbol) collection efficiencies of three nonwoven textiles: a) Quilters Dream Cotton, C1; b) Pellon Natural Cotton, C2; and c) Pellon Viscose Bamboo, BC. The standard deviation of the measured collection efficiency was small. The error bars representing one standard deviation fit within the symbol.

Table I

Titanium content measured by field portable x-ray florescence (FPXRF) for 11 nonwoven textiles.

Color	Brand Name, Identifier	Material	Mean FPXRF Titanium Result ^a (µg g ⁻¹)
White	Quilters Dream Poly Request Loft, P1	Polyester	11.9
White	Quilters Dream Puff, P2	Polyester	8.1
White	Pellon Polyester, P3	Polyester	7.8
White	Quilters Dream Blend Select Loft, CP	70% Cotton 30% Polyester	8.4
White	Quilters Dream Angel Request Loft, A1	Fire-Retardant Fibers	5.6
Black	Quilters Dream Poly Request Loft, P4	Polyester	8.6
Off-White	Quilters Dream Wool, W1	Wool	3.3
Off-White	Pellon Wool, W2	Wool	2.9
Off-White	Quilters Dream Cotton Request Loft, C1	Cotton	< LOD ^b
Off-White	Pellon Natural Cotton, C2	Cotton	< LOD ^b
Off-White	Pellon Viscose Bamboo Blend, BC	50% Bamboo 50% Cotton	< LOD ^b

^aThree measurements were taken for each test material.

^bThe LOD of the FPXRF is 0.15 µg/cm².

Bold indicates that the material was selected for further analysis. Quilters Dream textiles from Quilters Dream Batting, Virginia Beach, VA Pellon textiles from Pellon Consumer Products, Clearwater, FL

Characteristics of selected nonwoven textiles. Mean metals content of selected nonwoven textiles measured by inductively coupled plasma-optical emission spectroscopy (ICP-OES). Standard deviation of three measurements shown in parentheses. Data reported as ND were all below the detection limit.

Table II

Nonwoven Textile	Thickness ^a (mm)	Basis Weight (g m ⁻²)	Density (g cm ⁻³)	ICP-OES Metals Content (µg g ⁻¹)						
				Cr	Cu	Fe	Mn	Ti	Zn	
C1	1.75	99 (1.8)	1.52	–	1.2 (1.2)	42 (3.6)	25 (0.4)	6 (1.3)	15 (4.2)	
C2	3.28	187 (7.5)	1.52	0.9 (0.8)	9.9 (2.2)	127 (7.0)	49 (3.6)	21 (9.5)	34 (3.0)	
BC	1.59	104 (5.2)	1.51	1.7 (0.4)	5.3 (0.6)	65 (12.1)	24 (1.9)	14 (4.2)	214 (26)	
Nylon mesh ^b	–	–	–	1.0 (0.9)	ND	ND	2.5 (0.06)	812 (141)	0.6 (0.5)	

^aThickness of one layer

^bNylon mesh results are from Mines et al.⁽⁶⁾