



HHS Public Access

Author manuscript

Ann Work Expo Health. Author manuscript; available in PMC 2017 September 28.

Published in final edited form as:

Ann Work Expo Health. 2017 March 01; 61(2): 237–247. doi:10.1093/annweh/wxw020.

Confidence Intervals for Asbestos Fiber Counts: Approximate Negative Binomial Distribution

David Bartley^{1,*}, James Slaven², and Martin Harper³

¹Consultant, 3904 Pocahontas Avenue, Cincinnati, OH 45227, USA

²Department of Biostatistics, Indiana University School of Medicine, 340 W 10th St #6200, Indianapolis, IN 46202, USA

³Health Effects Laboratory Division, Exposure Assessment Branch, National Institute for Occupational Safety and Health, 1095 Willowdale Rd MS-3030, Morgantown, WV 26505, USA

Abstract

The negative binomial distribution is adopted for analyzing asbestos fiber counts so as to account for both the sampling errors in capturing only a finite number of fibers and the inevitable human variation in identifying and counting sampled fibers. A simple approximation to this distribution is developed for the derivation of quantiles and approximate confidence limits. The success of the approximation depends critically on the use of Stirling's expansion to sufficient order, on exact normalization of the approximating distribution, on reasonable perturbation of quantities from the normal distribution, and on accurately approximating sums by inverse-trapezoidal integration. Accuracy of the approximation developed is checked through simulation and also by comparison to traditional approximate confidence intervals in the specific case that the negative binomial distribution approaches the Poisson distribution. The resulting statistics are shown to relate directly to early research into the accuracy of asbestos sampling and analysis. Uncertainty in estimating mean asbestos fiber concentrations given only a single count is derived. Decision limits (limits of detection) and detection limits are considered for controlling false-positive and false-negative detection assertions and are compared to traditional limits computed assuming normal distributions.

Keywords

asbestos; fiber counting quality control; negative binomial confidence

* Author to whom correspondence should be addressed. Tel: +1-513-652-4949; bartleydavy@gmail.com.

Supplementary Data

Supplementary data are available at *Annals of Work Exposures and Health* online.

Conflict of Interest Statement

The authors declare no conflict of interest relating to the material presented in this article. Its contents, including any opinions and/or conclusions expressed, are solely those of the authors.

Introduction

Airborne asbestos fiber concentrations are often determined in terms of total fiber counts n obtained manually by counting fibers on a microscope slide within a specific area A (often 100 fields with total area 0.785 mm²). The value n differs from the true mean number N of fibers per area A , since the number of fibers to be counted in the finite area A varies around N . This variation follows the Poisson distribution. Furthermore, counter variation introduces uncertainty, leading to observations over-dispersed relative to the Poisson distribution where the variance equals the mean. A great variety of count data have been analyzed in this situation using the negative binomial distribution as extension of the Poisson distribution (for instance, see Cameron and Trivedi, 2013). This is the approach adopted in this paper.

Specifically, given a single count n , simple expressions for confidence limits enclosing the unknown N at specified probability are derived. Such limits are vital in establishing exceedance or, conversely, an upper bound on the true mean count. Furthermore, confidence in the presence or absence of fibers can be quantified.

Background

Confidence intervals about N

The earliest reported confidence intervals for asbestos fiber counting originated with an experiment at the Health and Safety Laboratory, Cricklewood, England (Ogden, 1982). The experiment provided data from 66 filters analyzed by ~10 counters with a variety of mean asbestos fiber counts N . These data were modeled with variance σ^2 approximated by:

$$\sigma^2 = N + s^2 N^2, \quad (1)$$

determining an estimate $s \approx 20\%$ representing the count variation at large N . The term in equation (1) linear in N represents Poisson variation in the number of fibers that appear within the microscope fields searched.

This value for s is consistent with a recent evaluation from Lee *et al.* (2015), who analyzed the capabilities of laboratory counters in the analysis of chrysotile fibers. Six slides were analyzed independently by seven laboratories, using a single counter in each. The slides were relocatable, meaning that identical fields were examined by each counter and that Poisson sampling error was absent. Oneway analysis of the data was carried out, assuming that (unknown) true counts for each slide were represented by consensus lab means and that inter-laboratory relative variances were approximately constant over the slides and therefore that the variance was estimable by their averages with $6 \cdot (7 - 1)$ degrees of freedom. The result was an inter-laboratory relative standard deviation equal to 22%. This figure is close to the intra-laboratory (in this case, inter-counter) estimate, 20%, found by Ogden (1982). How these figures would vary with asbestos type is unknown.

Confidence limits were determined (Ogden, 1982) by identifying an approximate pivot (i.e. a function of N whose distribution is known and is independent of N). The distribution of the function

$$\text{pivot}[n, N] \equiv (n - N) / \sqrt{N + s^2 N^2}, \quad (2)$$

where n are measured counts, was found to only weakly depend on N . The distribution of the ~660 values of the pivot in the Cricklewood experiment was plotted as in Fig. 1.

The graph is composed of a range of mean values N , and therefore, both right and left single-sided 95% confidence limits (-1.5, 2.0) can be read off from the graph. In other words, 95% of the measurements \hat{n} have

$$(n - N) / \sqrt{N + s^2 N^2} < 2.0, \quad (3a)$$

and 95% have:

$$(n - N) / \sqrt{N + s^2 N^2} > -1.5. \quad (3b)$$

Squaring both sides of the inequality in equation (3a) and in equation (3b) results in inequalities quadratic in N , which are easily solved for N in terms of functions—upper confidence limit, UCL[n], and lower confidence limit, LCL[n]—of single-count values n as:

$$N < \text{UCL}[n] \text{ at 95\% confidence,} \quad (4a)$$

and

$$N > \text{LCL}[n] \text{ at 95\% confidence,} \quad (4b)$$

where

$$\text{LCL}[n] = \frac{2\hat{n} + 2.0^2 - \sqrt{(2\hat{n} + 2.0^2)^2 - 4(1 - 2.0^2 s^2)n^2}}{2(1 - 2.0^2 s^2)} \quad (5a)$$

$$\text{UCL}[n] = \frac{2\hat{n} + 1.5^2 + \sqrt{(2\hat{n} + 1.5^2)^2 - 4(1 - 1.5^2 s^2)n^2}}{2(1 - 1.5^2 s^2)}. \quad (5b)$$

Note that NIOSH Method 7400 (NIOSH, 1994) and ASTM Method D7201 (ASTM, 2011) adopt the formalism presented above.

Limit of detection (decision limit) and detection limit

The limit of detection (LOD) is a figure defined to provide a means of limiting the false-positive rate (controlling ‘Type I errors’, null hypothesizing no significant asbestos fibers) in claiming the presence of a substance if actually absent or negligible. LOD can be defined as the bias-corrected signal level that is exceeded at probability $< 0.1\%$ when the substance is absent. Note that LOD as defined here is denoted a ‘decision limit’ by Currie (1984). Also, a ‘detection limit DL’ may be defined as the mean asbestos fiber density which gives a signal $> \text{LOD}$ at given confidence level [controlling false negatives (Type II errors)].

For many sampling/analytical methods the signal fluctuation approaches a constant as the presence of a substance becomes negligible. For example, in sampling unknown M (e.g. mass captured by a filter) the bias-corrected signal m may vary as:

$$m = M + \sqrt{\sigma_0^2 + M^2 s^2} \varepsilon, \quad (6)$$

where σ_0 is a constant and ε varies about zero with a normal distribution and unit variance. With the variance of the signal m given by:

$$\text{Var}[m] = \sigma_0^2 + M^2 s^2, \quad (7)$$

the constant s is therefore the ‘true relative standard deviation (i.e. the standard deviation relative to true values) for values of M large enough that the fractional difference

[equal to about $-\frac{1}{2}(\sigma_0/Ms)^2$] between s and $\sqrt{\sigma_0^2 + M^2 s^2}/M$ is negligible. In the limit $M \rightarrow 0$, the constant σ_0 determines the fluctuation, and LOD can be defined as:

$$\text{LOD} = 3 \times \sigma, \quad (8)$$

giving $\sim 0.1\%$ probability that $m > \text{LOD}$ if $M = 0$.

A value for LOD was published by NIOSH (1994), within NIOSH Method 7400 regarding asbestos fiber sampling and analysis using equation (8), even though equation (7) is not consistent with equation (1) at N small enough that the fractional difference (equal to about $-100\% + sN^{1/2}$) between Ns [from equation (7) at $\sigma_0 = 0$ and replacing M by N] and σ [equation (1)] is significantly negative. Furthermore, LOD was defined as the signal from asbestos fibers plus background filter fibers needed to claim the presence of at least an asbestos fiber at high confidence. The value was therefore ‘not’ bias corrected.

Specifically, in the development of NIOSH 7400, many counts n_i of interference fibers on blank filters indicated [with primes denoting densities (mm^{-2})] that

$$\text{Mean}[n'_i]=2.5 \text{ mm}^{-2}(N'_i) \left(\begin{array}{l} \text{N. Leidel, personal} \\ \text{communication} \end{array} \right)$$

$$\text{Variance}^{1/2}[n'_i]=1.5 \text{ mm}^{-2}. \quad (9)$$

Then, LOD_{7400} was taken to equal:

$$\text{LOD}_{7400}=N'_i+3 \text{ Variance}^{1/2}(n'_i)=2.5 \text{ mm}^{-2}+3 \times 1.5 \text{ mm}^{-2}=7 \text{ mm}^{-2}. \quad (10)$$

The term with factor 3 is as in equation (8), while the value 2.5 mm^{-2} refers to mean interference not related to the asbestos fibers sampled. Note that this value may be subtracted out from raw counts to give a bias-less signal if interfering fiber counts are stable. The quantitative difference between using equation (1) versus equation (7) is presented below in the section Applications.

Proposed

In this paper, we approach the issue of confidence intervals by adopting a specific distribution, namely the ‘negative binomial distribution’ [equation (A1)], rather than an empirically determined distribution as measured by Ogden (1982). As described in Supplementary Appendix A, available at *Annals of Work Exposures and Health* online, the negative binomial distribution is capable of describing the situation in which the variance σ^2 in a discrete variable n is given by equation (1) and for which the Poisson distribution results if $s \rightarrow 0$ (Johnson *et al.*, 1993). The negative binomial distribution then makes contact with the distribution of Ogden (1982) and is adopted here for analyzing the distribution of counts. Johnson *et al.* (1993) and Hilbe (2011) discuss the statistical adoption of the negative binomial distribution for modeling discrete random variables that ideally reflect the Poisson distribution, but which exhibit overdispersion.

In order to obtain useful expressions for the confidence intervals, an approximation to the negative binomial distribution is worked out. The details of this derivation are generally not of interest to those applying the results and are therefore relegated to Supplementary Appendix A, available at *Annals of Work Exposures and Health* online. The body of the paper then summarizes results, and the accuracy of the confidence intervals is derived.

Confidence Intervals

This paper develops simple single-sample confidence intervals surrounding population mean counts small enough that vestiges of the Poisson distribution are present. If larger counts are encountered, counting may be stopped at fewer than 100 fields. For example, Roggli *et al.* (1992) suggests stopping at 200 fibers. In such cases, Poisson-distribution effects are

negligible, and the relative standard deviation is approximately constant. This situation is not discussed further in the paper.

Approximate quantiles of the negative binomial distribution

We first consider simply the distribution quantile, namely the upper limit on a single count n at specified probability β (e.g. 95%) given measured counter variability s and specified mean count N . This limit may be defined for discrete (rather than continuous) random variables as follows. The (upper) quantile $n_\beta[N, s]$ is the smallest integer for which

$$\Pr[n \leq n_\beta] \geq \beta. \quad (11)$$

As derived in Supplementary Appendix A, available at *Annals of Work Exposures and Health* online, the quantile n_β for the negative binomial distribution after smoothing discrete discontinuities may be approximated simply as [equation (A22)]:

$$(n_\beta - N)/\sigma \approx z_\beta + \frac{1}{6}(z_\beta^2 - 1)(1 + 2Ns^2)/\sigma, \quad (12)$$

where σ is given by equation (1) and z_β is the normal-distribution quantile (e.g. $z_\beta = -1.645$ at $\beta = 0.05$ and $z_\beta = +1.645$ at $\beta = 0.95$).

Comparison of exact and approximate quantiles

So as to illustrate accuracy, the above approximating functions were plotted along with exact functions, computed numerically, in a number of circumstances. Deviation of the quantile from mean count N was plotted versus N and normalized as given by Ogden (1982) and as in equation (2) by dividing by $\sqrt{N + s^2 N^2}$ so as to plot a reasonable range on a single figure.

Figure 2 shows 5 and 95% quantiles at ‘true relative standard deviation s ’ equal to 20% (as with data of Ogden, 1982). Figure 3 shows quantiles at $s = 40\%$. Figure 4 presents comparisons for the Poisson distribution ($s = 0$).

Naturally, the approximations improve with decreasing s , considering the reliance on expansions [equation (A16)] about the mode of the probability distribution. Regardless, the accuracy is surprising in view of the simplicity of the approximating functions. Note that for some applications, only the averaging (indiscrete) quantiles of equation (A22) (also indicated in the figures) may be needed.

Single-sided confidence limits

Given the above simple expressions for the distribution quantile, we now consider confidence intervals limiting the true but unknown mean count N . Because of the discrete character of counts n (just as with the Poisson distribution), exact confidence limits at specified confidence do not exist. However, approximate limits result from the smoothed expression of equation (12), similar to the chi-square approximation for the Poisson distribution (Johnson *et al.*, 1993). Equation (12) indicates that n_β is an increasing function

of N . Therefore, a single-sided confidence limit on N can be determined by solving for $M[n_\beta, s]$. Then, equation (11) implies that

$$\Pr[N > N[n, s]] \approx \beta$$

Note that the count n , not N , is the random variable in equation (13), expressing the sense of a lower confidence limit, $LCL[n]$:

$$LCL[n] = N[n, s]. \quad (14)$$

The function $M[n_\beta, s]$ can be easily obtained by solving equation (12) for σ^2 , resulting in a quadratic equation in N upon using equation (1).

Yet simpler and useful is to break up the domain of interest into cases $s = 0$ (corresponding to the Poisson distribution) and $s > 0$ where an approximate pivot may be adopted (a function of N and n with distribution known and independent of N). Ogden (1982) considered as approximate pivot the function $(n - N)/\sigma[N]$ [equation (2)], with σ^2 given by equation (1) and where then ideally, with quantile n_β , $(n_\beta - N)/\sigma$ would be nearly independent of N .

The constancy of this function within the above approximation to the negative binomial distribution was determined by using the smoothed quantile \bar{n}_β [equation (A22)] and plotting $(\bar{n}_\beta - N)/\sigma$ versus N at various values of s (namely $s = 0, 20$, and 40%). The results are shown in Fig. 5.

Note that as N becomes large, equation (12) implies that

$$(n_\beta - N)/\sigma \rightarrow z_\beta + \frac{1}{3}(z_\beta^2 - 1)s \equiv l_\beta, N \gg 1, \quad (15)$$

which clarifies the approximate pivot of equation (2) (Ogden, 1982). Figure 5 indicates that the normalized quantile [the left-hand side of equation (15)] rapidly approaches the limit l_β as N increases if $s = 20\%$. This means that $M[n_\beta, s]$ may be approximated by simply solving equation (15) for N (by squaring both sides and solving the quadratic equation). The result, eliminating a spurious root, is:

$$LCL[n] = \frac{2n + l_\beta^2 - \sqrt{(2n + l_\beta^2)^2 - 4(1 - l_\beta^2 s^2)n^2}}{2(1 - l_\beta^2 s^2)}. \quad (16a)$$

The same reasoning yields an upper single-sided confidence limit $UCL[n]$ at probability, β (e.g. 95%):

$$UCL[n] = \frac{2n + l_{1-\beta}^2 + \sqrt{(2n + l_{1-\beta}^2)^2 - 4(1 - l_{1-\beta}^2 s^2)n^2}}{2(1 - l_{1-\beta}^2 s^2)}, \quad (16b)$$

noting the sign change in front of the square root. The above expressions also result in two-sided confidence intervals in the sense that:

$$\Pr[LCL[n] < N < UCL[n]] \approx 2\beta - 1 \text{ (e. g. } 95\%, \text{ if } \beta=0.975) \quad (17)$$

The Poisson distribution (at $s = 0$) is obtained using equation (12) directly. Details are given in Supplementary Appendix A, available at *Annals of Work Exposures and Health* online. Comparison is made to traditional confidence intervals involving a relation to the chi-square distribution.

Simulations

In order to judge the accuracy of the above expressions when applied to discrete random variables, many simulations were carried out. At each of mean number, $N = 5.1, 5.1, \dots, 30$, a random number generator produced 10 000 negative binomial distributed values for checking the above inequalities. Results are given in Figs 6 and 7 for $s = 20\%$ and $s = 40\%$.

If strict confidence limits existed, the data would fall close to horizontal straight lines. The scatter about these lines is evident in Figs 6 and 7. However, the scatter is strictly limited. In fact, the limits $\lim[N]$ in the single-sided case may be approximated by considering how the confidence level β must change in order to increase the quantile n_β of equation (12) by 1. The result is that:

$$\lim[N] \approx \beta \pm \frac{1/2}{\left(1 + \frac{1}{3} z_\beta s\right) \sqrt{2\pi} \text{Exp}[z_\beta^2/2] \sigma[N]}, \quad (18)$$

where $\sigma[N]$ is given by equation (1). The two-sided case of equation (18) is approximated by summation, as the upper and lower frequencies are generally not commensurate.

Note that though scatter is significant, no bias is evident in the confidence levels. The effect of discrete scatter on confidence limits can be estimated by computing the shifts in equation (16) induced by shifts in β . For example, at $s = 20\%$ and $N = 10$, the upper confidence limit shifts by only about $\pm 5\%$.

A further set of simulations was carried out, solving equation (12) for N exactly, rather than using the pivot as in equation (15). The results differ insignificantly from Figs 6 and 7. We conclude that at least for $s \geq 20\%$, the simpler expressions of equation (16) are adequate.

Applications

Derivation of the early intuitive confidence limits

One application of the negative binomial formulism is derivation of the results published by Ogden (1982). This is done directly using equation (15). At $s = 20\%$, equation (15) indicates that

$$(n_{0.95} - N)/\sigma \rightarrow z_{0.95} + \frac{1}{3}(z_{0.95}^2 - 1)s = 1.8, \quad \text{and} \quad (n_{0.05} - N)/\sigma \rightarrow z_{0.05} + \frac{1}{3}(z_{0.05}^2 - 1)s = -1.5.$$

(19)

The limits $(-1.5, 1.8)$ are consistent with the published values $(-1.5, 2.0)$, noting that very few experimental data points were available at large mean count N . Agreement with experiment thus lends support to the utility of the negative binomial distribution.

Uncertainty

Limits $(-1.8, 2.1)$ at the 97.5% level may be obtained by replacing 1.645 by 1.960 in equation (19). This results in 95% confidence limits are given by equation (16) as indicated in Fig. 8.

The expanded uncertainty (ISO Guide 98-3:2008) in an estimate of N on the basis of a single count can be read directly from this figure, with the understanding that the uncertainty is unusual in its asymmetry about zero. Note that with interfering fibers present on sampling filters, fibers present and variable on filters (e.g. blanks) prior to sampling which may affect false-positive rates, the above confidence limits refer to 'total' mean fiber numbers in a given area, rather than specifically asbestos fibers. A table of lower and upper two-sided 95% confidence limits is given in Table 1 (and the values can be compared with the similar table in HSG248, 2005).

Limit of detection (decision limit) and detection limit

Specification of LOD can be improved over NIOSH Method 7400 by using the negative binomial distribution rather than the normal approximation of equations (8) and (10). Description of the experimental design that resulted in the variance in equation (9) no longer exists. For instance, it is not known whether exactly 100 fields were always examined or whether the filters came from different batches. The mean value, however, given in equation (9) is less problematic. In the following, the above mean value is accepted, whereas the variance is computed assuming intra-laboratory relative standard deviation for large counts is approximated as 20% as from the experiments of Ogden (1982).

The standard deviation arising from considering count variance in a sample of area A may be calculated as:

$$\text{Variance}[n_a+n_i]=(N_a+N_i)+s^2(N_a+N_i)^2, \quad (20)$$

with $s = 20\%$, and with the mean background count density N'_i taken as 2.5 mm^{-2} , as in equation (20). Setting N_a to zero and $A = 0.785 \text{ mm}^2$ for 100 fields, results in

$$\text{Variance}^{1/2}[n'_i]=\sqrt{N'_i/A+s^2N_i'^2}=1.85 \text{ mm}^{-2}, \quad (21)$$

a result not inconsistent with the value 1.5 mm^{-2} , especially if a variety of filter areas was sometimes assessed. The variation, filter to filter, in the number of interfering fibers was evidently found insignificant relative to the uncertainty in reading them. Henceforth, the figure 1.5 mm^2 is ignored aside from indicating consistency.

The cumulative negative binomial distribution and normal distribution giving equation (20) are illustrated in Fig. 9 at $N'_a=0$, TRSD = 20%, $N'_i=2.5 \text{ mm}^{-2}$, and $A = 0.785 \text{ mm}^2$.

Now the quantile at confidence equal to 0.999 is easily computed for the negative binomial distribution with the result:

$$(n'_iA)_{0.999}=8. \quad (22)$$

Thus, finally, LOD is given by:

$$\text{LOD}=(n'_iA)_{0.999}/A - N'_i=7.7 \text{ mm}^{-1} \quad (\text{at } A=0.785 \text{ mm}^2). \quad (23)$$

This value compares to

$$\text{LOD}_{\text{normal}}=4.5 \text{ mm}^{-2} \quad (24)$$

[which is identical to $\text{LOD}_{7400} = 7 \text{ mm}^{-2}$, remembering that the values in equations (24) and (25) refer to bias-less signals (unlike the published NIOSH value)]. The meaning of LOD is that the probability < 0.001 that the signal $> 7.7 \text{ mm}^2$ in the case of negligibly sampled asbestos. In other words, the false-positive rate in claiming the presence of asbestos is < 0.001 if 7.7 mm^2 is taken as the threshold value for making such a claim. Note that the claimed confidence level equal to 0.999 may be misleading in view of uncertainty in the distribution of interfering non-asbestos fibers present on the sampling filters. How to handle this source of uncertainty in terms of prediction intervals is described in ISO 15767 (2009).

Analysis using the negative binomial distribution therefore is seen to give a qualitatively distinct result from the usual normal assumptions for computing the limit of detection. Calculation of a detection limit DL (for controlling false negatives) would similarly differ.

Calculation as above indicates that $DL = 12 \text{ mm}^{-2}$ (~10 counts in 0.785 mm^2) at 80% confidence.

Conclusions

A simple approximation to the negative binomial distribution has been developed. The aim has been the statistical analysis of asbestos fiber counts accounting for Poisson variation associated with errors in sampling a finite number of fibers as well as counter variability in analysis. This approach has been shown to connect with early studies of count statistics reported by Ogden (1982). Estimation of the uncertainty in measuring a mean fiber concentration given a single count has been established. Specification of upper or lower confidence limits on fiber concentrations is also possible, relevant to proving that an occupational exposure limit has or has not been exceeded.

Decision and detection limits for specifying false-positive and false-negative detection rates are also possible. Traditional specification using the normal distribution is shown to differ significantly from accounting for the discrete sampling problem. For example, the decision limit computed from the negative binomial distribution is found to be almost twice as large as from the normal distribution.

The negative binomial approximation is so simple that other applications are no doubt possible. For example, perhaps analysis of how best to use field blanks so as to minimize the effect of spurious fibers is feasible. The variety of possible applications and corresponding experimental designs is large, as seen in disparate approaches of sampling and analysis described in NIOSH 7400, ASTM 7201, HSG 248, and ISO 8672. Simplicity in the statistical analysis is vital.

Supplementary Material

Refer to Web version on PubMed Central for supplementary material.

Acknowledgments

Funding

Health Effects Laboratory Division, National Institute for Occupational Safety and Health, Centers for Disease Control and Prevention (Project No. 927001Q) to D.B. and J.S.

References

- ASTM D7201. Standard practice for sampling and counting airborne fibers, including asbestos fibers, in the workplace, by phase contrast microscopy (with an option of transmission electron microscopy). West Conshohocken, PA: ASTM International; 2011.
- Cameron, AC., Trivedi, PK. Regression analysis of count data. 2nd. Cambridge, UK: Cambridge University Press; 2013.
- Currie, LA. Lower limit of detection: definition and elaboration of a proposed position for radiological effluent and environmental measurements. Springfield, VA: National Bureau of Standards Report available from U.S Government Printing Office, through National Technical Information Service; 1984.
- Hilbe, JM. Negative binomial regression. Cambridge, UK: Cambridge University Press; 2011.

- HSG248. Asbestos: the analysts' guide for sampling, analysis and clearance procedures. London, UK: Health and Safety Executive; 2005.
- ISO 8672. Air quality—determination of the number concentration of airborne inorganic fibres by phase contrast optical microscopy—membrane filter method. Geneva, Switzerland: International Organization for Standardization; 2014.
- ISO 15767. Workplace atmospheres—controlling and characterizing uncertainty in weighing collected aerosols. Geneva, Switzerland: International Organization for Standardization; 2009.
- ISO Guide 98-3. Uncertainty of measurement—part 3: guide to the expression of uncertainty in measurement (GUM:1995). Geneva, Switzerland: International Organization for Standardization; 2008.
- Johnson, NL., Kotz, S., Kemp, AW. Univariate discrete distributions. New York, NY: John Wiley & Sons; 1993.
- Lee EG, Nelson JH, Kashon ML, et al. Evaluation of the dark-medium objective lens in counting asbestos fibers by phase-contrast microscopy. *Ann Occup Hyg.* 2015; 59:616–628. [PubMed: 25737333]
- NIOSH Method 7400. Asbestos and other fibers by PCM. NIOSH manual of analytical methods (NMAM). 4th. Cincinnati, OH: National Institute for Occupational Safety and Health (NIOSH); 1994.
- Ogden, TL. The reproducibility of asbestos counts. London, UK: Health and Safety Executive; 1982. Health and Safety Executive Research Paper 18
- Roggli, VL, Greenberg, SD., Pratt, PC., editors. Pathology of asbestos associated disease. Boston, MA: Little Brown; 1992.




Figure 1. Distribution of $pivot[N]$ from the Cricklewood experiment ($M = N$). Solid circles include all the data, whereas open circles refer to $N < 5$, and 'x' to $N > 25$ and indicate rough independence of the distribution on N (UK Crown Copyright, 1982; reproduced from Ogden, 1982, by permission).




Figure 2.

Normalized negative binomial quantiles $-(n_\beta - N) / \sqrt{N + s^2 N^2}$ for large- N true relative standard deviation $s = 20\%$ at levels $\beta = 5$ and 95% plotted versus population mean count N . Exact values (blue); approximations [red, equation (A21)] shifted slightly left for graphical visibility; smooth curve [red, equation (A22)] neglecting the discontinuities of the discrete values.




Figure 3. Normalized negative binomial quantiles at $s = 40\%$ at levels $\beta = 5$ and 95% plotted versus population mean count N . Exact values (blue); approximations (red).




Figure 4. Normalized Poisson distribution quantiles at levels $\beta = 5$ and 95% plotted versus population mean count N . Exact values (blue); approximations (red).




Figure 5. Normalized 95% quantiles versus the mean N at several values of true relative standard deviation s . The horizontal lines represent asymptotic values l_β at $N \rightarrow \infty$.

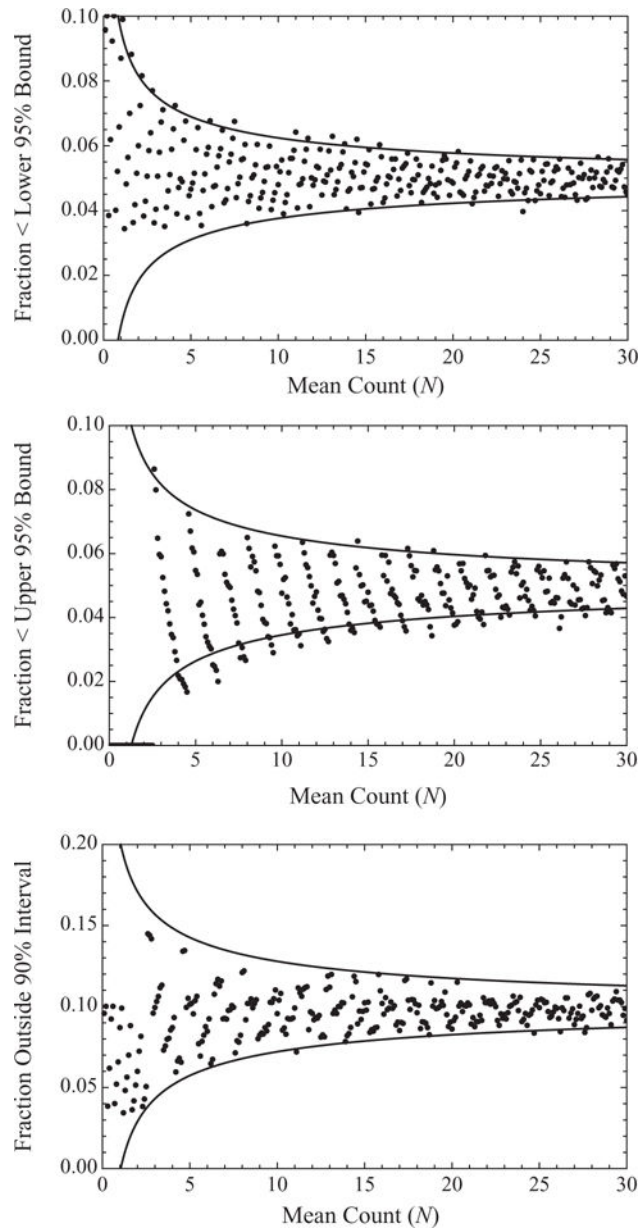


Figure 6. Negative binomial confidence interval levels at $s = 20\%$ at nominal single-sided levels = 5% and two-sided interval with nominal level = 10%. Solid curves are approximate limits on the discrete variation [equation (18)].

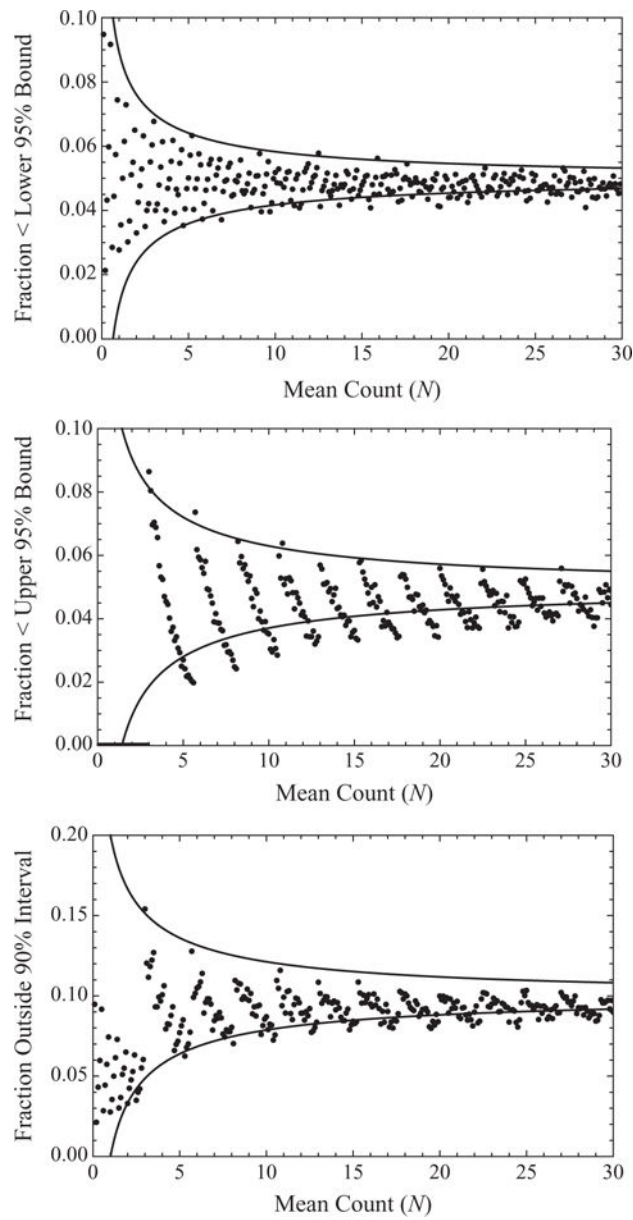


Figure 7. Negative binomial confidence interval levels at $s = 40\%$. Solid curves are approximate limits on the discrete variation [equation (18)].




Figure 8. Relative [i.e. $(n_{\beta} - n)/n \times 100\%$] confidence limits at the 95% level at intra-lab imprecision $s = 0.20$.




Figure 9. Cumulative normal and negative binomial distributions of background counts in 100 fields, assuming the mean value $N'_i=2.5 \text{ mm}^{-2}$ as published in NIOSH 7400 and intra-counter variability = 20%. The LOD values indicated refer to bias-less signals from a single filter, i.e., with 2.5 mm^2 subtracted out.

Table 1

Lower and upper two-sided 95% confidence limits (CL). Standard deviation (RSD) relative to count approaches 20% in large-count limit. Values at count < 5 as derived from an asymptotic continuum model are only suggestive.

Count	RSD (%)	Lower CL	Upper CL
1	102	0	6
3	61	1	10
5	49	2	13
7	43	3	16
10	37	5	21
20	30	11	37
50	24	32	85
100	22	67	163
200	21	137	319

Author Manuscript

Author Manuscript

Author Manuscript

Author Manuscript