



1 Supplemental figure

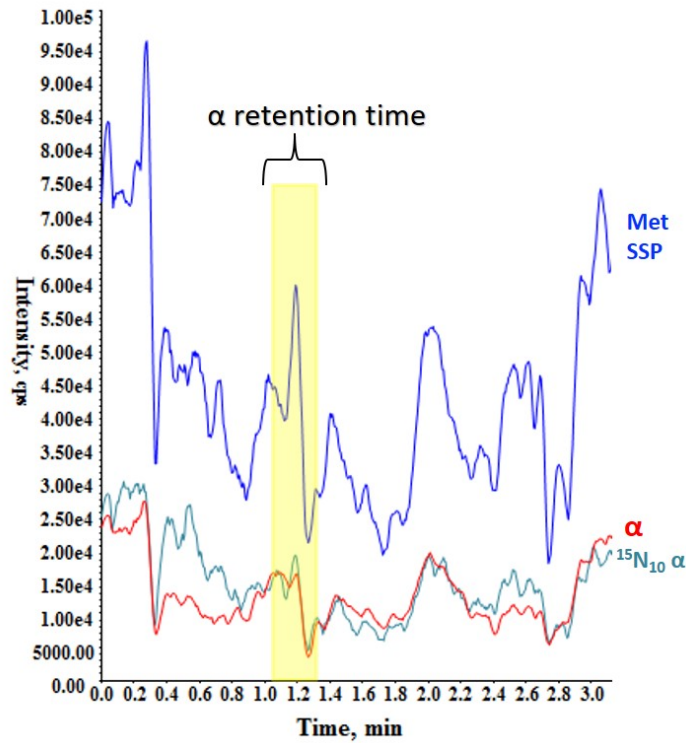

2

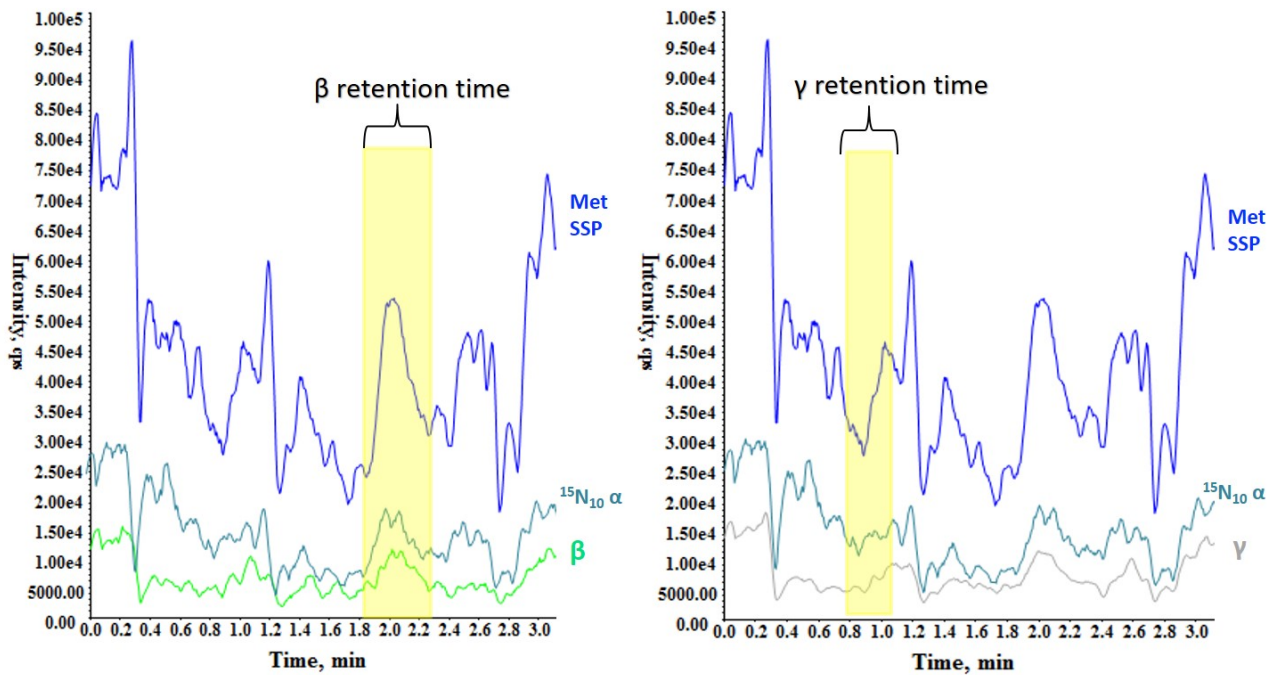

3

4

5 **Supplemental Figure 1.** Post column infusion chromatograms of the two different candidate internal
6 standards ($^{15}\text{N}_{10}$ - α -amanitin and methoinine sulfoxide synthetic peptide [MetSSP]) with each analyte (α -
7 β -, and γ -amanitin) in one individual urine matrix. The expected retention time for each analyte is
8 highlighted in yellow.

9

10

11